

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018995.D
 Acq On : 20 Oct 2020 03:31
 Operator : SY/MD
 Sample : L4430-09DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB2	254398	262558	21.33%	2.299%
2	1.579	144	152	165	rBV	136922	155547	12.64%	1.362%
3	2.122	311	321	348	rVB	259434	413048	33.56%	3.617%
4	2.441	418	420	423	rBV3	523	353	0.03%	0.003%
5	2.782	517	526	540	rVB3	9400	17051	1.39%	0.149%
6	2.955	578	580	582	rBV	591	298	0.02%	0.003%
7	3.077	615	618	621	rBV2	458	300	0.02%	0.003%
8	3.184	649	651	652	rBV	315	139	0.01%	0.001%
9	3.257	672	674	677	rBV	249	140	0.01%	0.001%
10	3.328	693	696	702	rVB3	443	397	0.03%	0.003%
11	3.360	702	706	708	rBV2	288	254	0.02%	0.002%
12	3.421	720	725	726	rBV2	350	245	0.02%	0.002%
13	3.434	726	729	731	rBV	380	218	0.02%	0.002%
14	3.647	791	795	798	rBV3	440	488	0.04%	0.004%
15	3.839	852	855	857	rBV2	295	218	0.02%	0.002%
16	3.936	866	885	917	rBV2	401393	1162241	94.42%	10.176%
17	4.376	1007	1022	1050	rBV	200918	497712	40.43%	4.358%
18	4.753	1137	1139	1140	rBV2	492	163	0.01%	0.001%
19	4.907	1185	1187	1188	rVB2	416	98	0.01%	0.001%
20	5.071	1221	1238	1269	rBV2	476003	1230928	100.00%	10.778%
21	5.431	1348	1350	1352	rVB3	470	234	0.02%	0.002%
22	5.556	1386	1389	1392	rVB	510	316	0.03%	0.003%
23	5.640	1402	1415	1448	rBV	374421	750227	60.95%	6.569%
24	5.936	1492	1507	1534	rBV3	317498	672050	54.60%	5.884%
25	6.093	1543	1556	1582	rBV	278516	567628	46.11%	4.970%
26	6.335	1628	1631	1635	rBV2	663	470	0.04%	0.004%
27	6.360	1635	1639	1641	rBV2	431	330	0.03%	0.003%
28	6.476	1673	1675	1677	rBV	197	115	0.01%	0.001%
29	6.643	1724	1727	1728	rBV	287	147	0.01%	0.001%
30	6.736	1752	1756	1759	rVB3	543	314	0.03%	0.003%
31	6.781	1767	1770	1774	rBV2	255	157	0.01%	0.001%
32	6.881	1799	1801	1802	rBV	352	169	0.01%	0.001%
33	6.939	1816	1819	1821	rBV2	244	178	0.01%	0.002%
34	7.010	1830	1841	1866	rBV	138718	253682	20.61%	2.221%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018995.D
 Acq On : 20 Oct 2020 03:31
 Operator : SY/MD
 Sample : L4430-09DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	7.338	1929	1943	1965	rBV	474320	815104	66.22%	7.137%
36	7.643	2028	2038	2058	rBV	94788	166565	13.53%	1.458%
37	7.814	2089	2091	2093	rBV2	251	120	0.01%	0.001%
38	7.997	2134	2148	2173	rBV	617941	1031222	83.78%	9.029%
39	8.109	2173	2183	2220	rVV2	269923	557340	45.28%	4.880%
40	8.463	2291	2293	2296	rBV2	202	78	0.01%	0.001%
41	8.521	2308	2311	2313	rVB	444	252	0.02%	0.002%
42	8.537	2313	2316	2319	rVB3	690	375	0.03%	0.003%
43	8.553	2319	2321	2322	rVB	233	60	0.00%	0.001%
44	8.566	2322	2325	2328	rBV	534	316	0.03%	0.003%
45	8.627	2341	2344	2346	rBV2	349	223	0.02%	0.002%
46	8.640	2346	2348	2350	rVV	306	95	0.01%	0.001%
47	8.707	2367	2369	2372	rBV2	192	119	0.01%	0.001%
48	8.736	2376	2378	2381	rVB	355	155	0.01%	0.001%
49	8.785	2391	2393	2397	rVB	428	250	0.02%	0.002%
50	8.810	2397	2401	2403	rBV	307	246	0.02%	0.002%
51	8.871	2408	2420	2444	rBV	527568	856260	69.56%	7.497%
52	9.132	2498	2501	2507	rBV3	391	343	0.03%	0.003%
53	9.199	2520	2522	2526	rVB2	346	238	0.02%	0.002%
54	9.232	2529	2532	2533	rBV	257	132	0.01%	0.001%
55	9.280	2545	2547	2549	rVB2	409	156	0.01%	0.001%
56	9.322	2556	2560	2562	rVB2	332	212	0.02%	0.002%
57	9.379	2575	2578	2581	rBV	366	279	0.02%	0.002%
58	9.424	2589	2592	2594	rBV2	292	207	0.02%	0.002%
59	9.547	2626	2630	2631	rBV	226	161	0.01%	0.001%
60	9.576	2637	2639	2641	rVB2	137	51	0.00%	0.000%
61	9.595	2641	2645	2647	rBV2	264	207	0.02%	0.002%
62	9.659	2663	2665	2668	rBV	427	217	0.02%	0.002%
63	9.685	2670	2673	2675	rVV	212	108	0.01%	0.001%
64	9.746	2689	2692	2696	rVB2	482	368	0.03%	0.003%
65	9.768	2696	2699	2700	rBV	362	164	0.01%	0.001%
66	9.804	2708	2710	2712	rBV	41	17	0.00%	0.000%
67	9.817	2712	2714	2717	rVB2	118	64	0.01%	0.001%
68	9.836	2717	2720	2721	rBV	324	180	0.01%	0.002%
69	9.910	2740	2743	2749	rBV	368	364	0.03%	0.003%
70	9.961	2756	2759	2761	rBV	203	136	0.01%	0.001%
71	10.084	2794	2797	2800	rBV2	297	193	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018995.D
 Acq On : 20 Oct 2020 03:31
 Operator : SY/MD
 Sample : L4430-09DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	10.170	2822	2824	2827	rBV	206	166	0.01%	0.001%
73	10.238	2833	2845	2866	rVB	275837	437687	35.56%	3.832%
74	10.312	2866	2868	2873	rBV2	503	386	0.03%	0.003%
75	10.350	2878	2880	2884	rVB2	349	222	0.02%	0.002%
76	10.373	2884	2887	2888	rBV2	308	190	0.02%	0.002%
77	10.482	2919	2921	2926	rVB2	210	171	0.01%	0.001%
78	10.630	2962	2967	2970	rBV	470	320	0.03%	0.003%
79	10.739	2999	3001	3004	rBV2	276	179	0.01%	0.002%
80	10.855	3034	3037	3040	rBV	190	162	0.01%	0.001%
81	10.894	3047	3049	3050	rBV	189	103	0.01%	0.001%
82	10.971	3071	3073	3075	rBV	193	98	0.01%	0.001%
83	11.270	3155	3166	3188	rBV	501735	768417	62.43%	6.728%
84	11.553	3252	3254	3257	rBV	312	182	0.01%	0.002%
85	11.646	3271	3283	3309	rBV	501954	789778	64.16%	6.915%
86	11.801	3330	3331	3333	rBV2	283	121	0.01%	0.001%
87	11.833	3339	3341	3345	rBB3	488	238	0.02%	0.002%
88	11.874	3352	3354	3355	rBV	287	114	0.01%	0.001%
89	12.257	3469	3473	3476	rBV	339	331	0.03%	0.003%
90	12.672	3599	3602	3603	rBV	301	167	0.01%	0.001%
91	12.807	3641	3644	3648	rBV	398	280	0.02%	0.002%
92	12.916	3675	3678	3682	rBV	312	261	0.02%	0.002%
93	12.990	3699	3701	3706	rVB	351	278	0.02%	0.002%


Sum of corrected areas: 11420841

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018995.D
Acq On : 20 Oct 2020 03:31
Operator : SY/MD
Sample : L4430-09DL 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

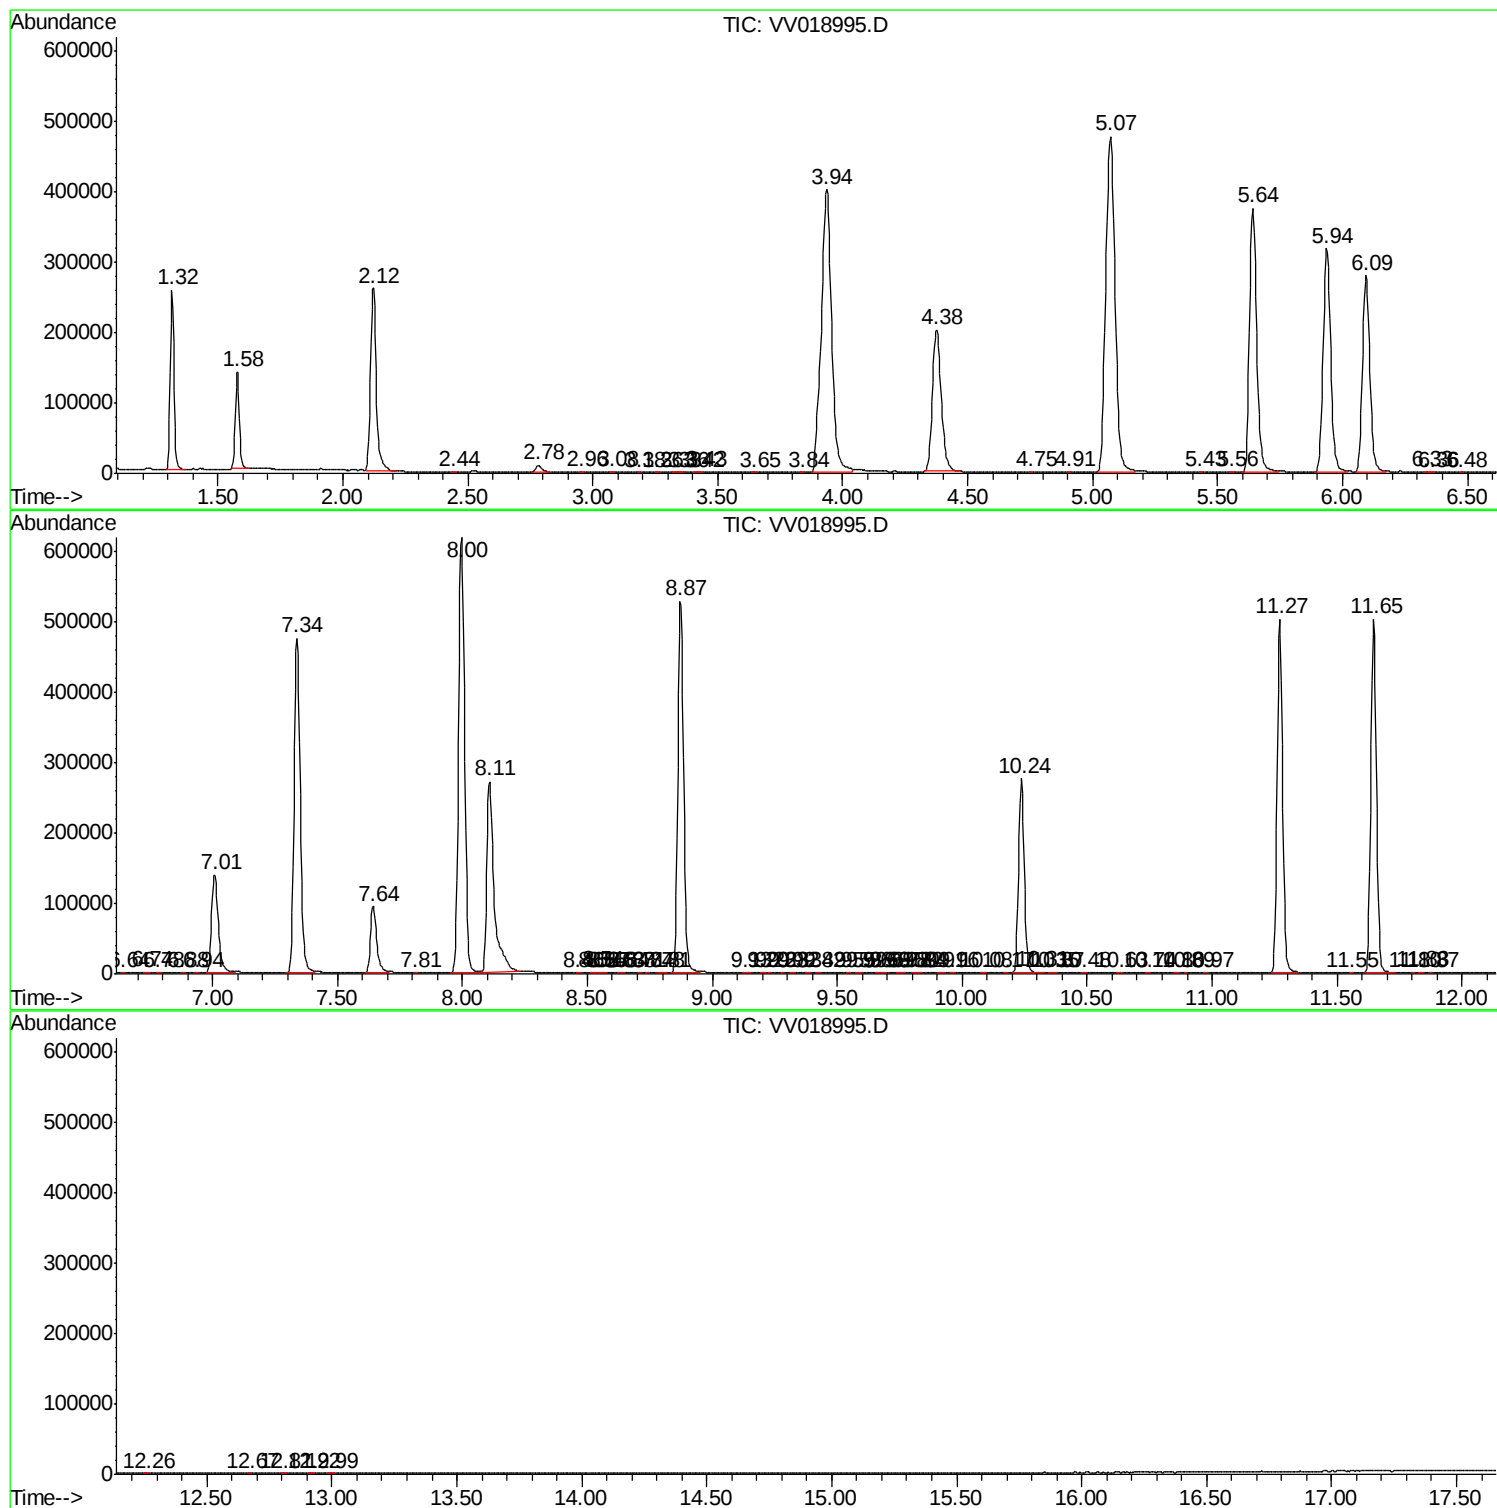

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018995.D
Acq On : 20 Oct 2020 03:31
Operator : SY/MD
Sample : L4430-09DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101920\
Data File : VV018995.D
Acq On : 20 Oct 2020 03:31
Operator : SY/MD
Sample : L4430-09DL 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AC0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
