

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018996.D
 Acq On : 20 Oct 2020 03:55
 Operator : SY/MD
 Sample : L4430-10 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	81	rVB	138937	139115	12.89%	1.696%
2	1.576	145	151	163	rVB	138053	150471	13.94%	1.835%
3	2.119	311	320	348	rVB	244353	383585	35.54%	4.677%
4	3.039	604	606	607	rBV	479	241	0.02%	0.003%
5	3.293	682	685	686	rBV	285	174	0.02%	0.002%
6	3.479	741	743	748	rBV2	332	323	0.03%	0.004%
7	3.553	762	766	767	rBV2	420	268	0.02%	0.003%
8	3.608	781	783	785	rBV2	285	134	0.01%	0.002%
9	3.659	797	799	801	rBV2	379	190	0.02%	0.002%
10	3.807	839	845	847	rBV2	435	499	0.05%	0.006%
11	3.907	865	876	900	rBV	95259	271437	25.15%	3.310%
12	4.373	1007	1021	1046	rBV	185105	457810	42.42%	5.582%
13	4.563	1077	1080	1082	rBV3	504	363	0.03%	0.004%
14	4.762	1139	1142	1146	rBV4	671	589	0.05%	0.007%
15	4.933	1192	1195	1200	rVB3	348	298	0.03%	0.004%
16	4.962	1200	1204	1206	rBV3	330	178	0.02%	0.002%
17	5.071	1222	1238	1261	rBV2	418976	1079243	100.00%	13.160%
18	5.267	1298	1299	1302	rVB	814	288	0.03%	0.004%
19	5.309	1309	1312	1316	rBV	439	360	0.03%	0.004%
20	5.393	1337	1338	1341	rVB2	347	156	0.01%	0.002%
21	5.421	1344	1347	1351	rBV3	343	276	0.03%	0.003%
22	5.640	1403	1415	1439	rBV	333123	662449	61.38%	8.077%
23	5.926	1493	1504	1522	rBV2	44773	93617	8.67%	1.142%
24	6.093	1543	1556	1579	rBV	252573	511567	47.40%	6.238%
25	6.399	1648	1651	1652	rBV	304	161	0.01%	0.002%
26	6.457	1667	1669	1677	rVB2	449	259	0.02%	0.003%
27	6.486	1677	1678	1679	rBV	143	41	0.00%	0.000%
28	6.505	1681	1684	1690	rVB2	367	301	0.03%	0.004%
29	6.598	1709	1713	1720	rBV3	330	372	0.03%	0.005%
30	6.650	1727	1729	1731	rBV	286	148	0.01%	0.002%
31	6.727	1750	1753	1760	rVB4	372	412	0.04%	0.005%
32	6.817	1778	1781	1783	rBV2	318	201	0.02%	0.002%
33	6.849	1787	1791	1792	rBV	292	183	0.02%	0.002%
34	6.901	1805	1807	1812	rVB	538	352	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018996.D
 Acq On : 20 Oct 2020 03:55
 Operator : SY/MD
 Sample : L4430-10 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.923	1812	1814	1821	rBV2	273	342	0.03%	0.004%
36	7.007	1829	1840	1869	rBV	125280	230210	21.33%	2.807%
37	7.338	1930	1943	1967	rBV	451261	777321	72.02%	9.478%
38	7.643	2028	2038	2061	rBV	92059	160531	14.87%	1.957%
39	7.875	2107	2110	2117	rVB	416	360	0.03%	0.004%
40	7.907	2117	2120	2122	rVB2	521	274	0.03%	0.003%
41	7.933	2122	2128	2129	rBV	286	237	0.02%	0.003%
42	8.000	2139	2149	2158	rBV7	4394	6735	0.62%	0.082%
43	8.036	2158	2160	2161	rBV7	227	74	0.01%	0.001%
44	8.109	2172	2183	2220	rBV2	257899	545094	50.51%	6.647%
45	8.437	2283	2285	2286	rBV2	264	140	0.01%	0.002%
46	8.563	2321	2324	2329	rBV2	378	371	0.03%	0.005%
47	8.746	2379	2381	2384	rBV	351	219	0.02%	0.003%
48	8.801	2387	2398	2400	rBV3	741	936	0.09%	0.011%
49	8.871	2409	2420	2446	rBV	504453	816961	75.70%	9.962%
50	9.093	2486	2489	2490	rBV	355	138	0.01%	0.002%
51	9.106	2491	2493	2496	rVB2	289	106	0.01%	0.001%
52	9.126	2497	2499	2502	rBV	348	211	0.02%	0.003%
53	9.206	2522	2524	2530	rVV2	325	163	0.02%	0.002%
54	9.238	2531	2534	2538	rVB2	436	340	0.03%	0.004%
55	9.643	2654	2660	2664	rBV2	476	449	0.04%	0.005%
56	9.662	2664	2666	2667	rBV2	236	74	0.01%	0.001%
57	9.781	2700	2703	2706	rBV2	310	176	0.02%	0.002%
58	9.820	2712	2715	2717	rBV	221	128	0.01%	0.002%
59	9.836	2717	2720	2723	rVB2	355	199	0.02%	0.002%
60	9.884	2729	2735	2740	rBV2	636	798	0.07%	0.010%
61	9.916	2742	2745	2750	rVB2	513	469	0.04%	0.006%
62	9.942	2751	2753	2756	rVB2	376	211	0.02%	0.003%
63	9.968	2756	2761	2762	rBV	313	277	0.03%	0.003%
64	10.032	2778	2781	2784	rBV2	234	134	0.01%	0.002%
65	10.238	2833	2845	2865	rBV	268091	421326	39.04%	5.137%
66	10.389	2888	2892	2894	rBV2	307	301	0.03%	0.004%
67	10.518	2930	2932	2936	rVB2	326	200	0.02%	0.002%
68	10.605	2955	2959	2961	rBV2	388	216	0.02%	0.003%
69	10.778	3010	3013	3016	rBV	417	277	0.03%	0.003%
70	10.842	3031	3033	3034	rBV	206	68	0.01%	0.001%
71	10.961	3068	3070	3073	rBV2	333	176	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018996.D
Acq On : 20 Oct 2020 03:55
Operator : SY/MD
Sample : L4430-10 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC1

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis

72	11.142	3123	3126	3129	rVB2	439	290	0.03%	0.004%
73	11.219	3147	3150	3152	rBV2	432	275	0.03%	0.003%
74	11.270	3155	3166	3190	rVV	473662	721660	66.87%	8.799%
75	11.412	3205	3210	3214	rBV3	474	559	0.05%	0.007%
76	11.547	3250	3252	3256	rBV	386	321	0.03%	0.004%
77	11.646	3271	3283	3301	rBV	480664	754849	69.94%	9.204%
78	11.916	3364	3367	3371	rVB2	502	342	0.03%	0.004%
79	11.939	3371	3374	3375	rBV	309	162	0.02%	0.002%
80	11.977	3383	3386	3387	rBV	282	167	0.02%	0.002%
81	12.309	3486	3489	3491	rBV2	392	249	0.02%	0.003%


Sum of corrected areas: 8201177

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018996.D
Acq On : 20 Oct 2020 03:55
Operator : SY/MD
Sample : L4430-10 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

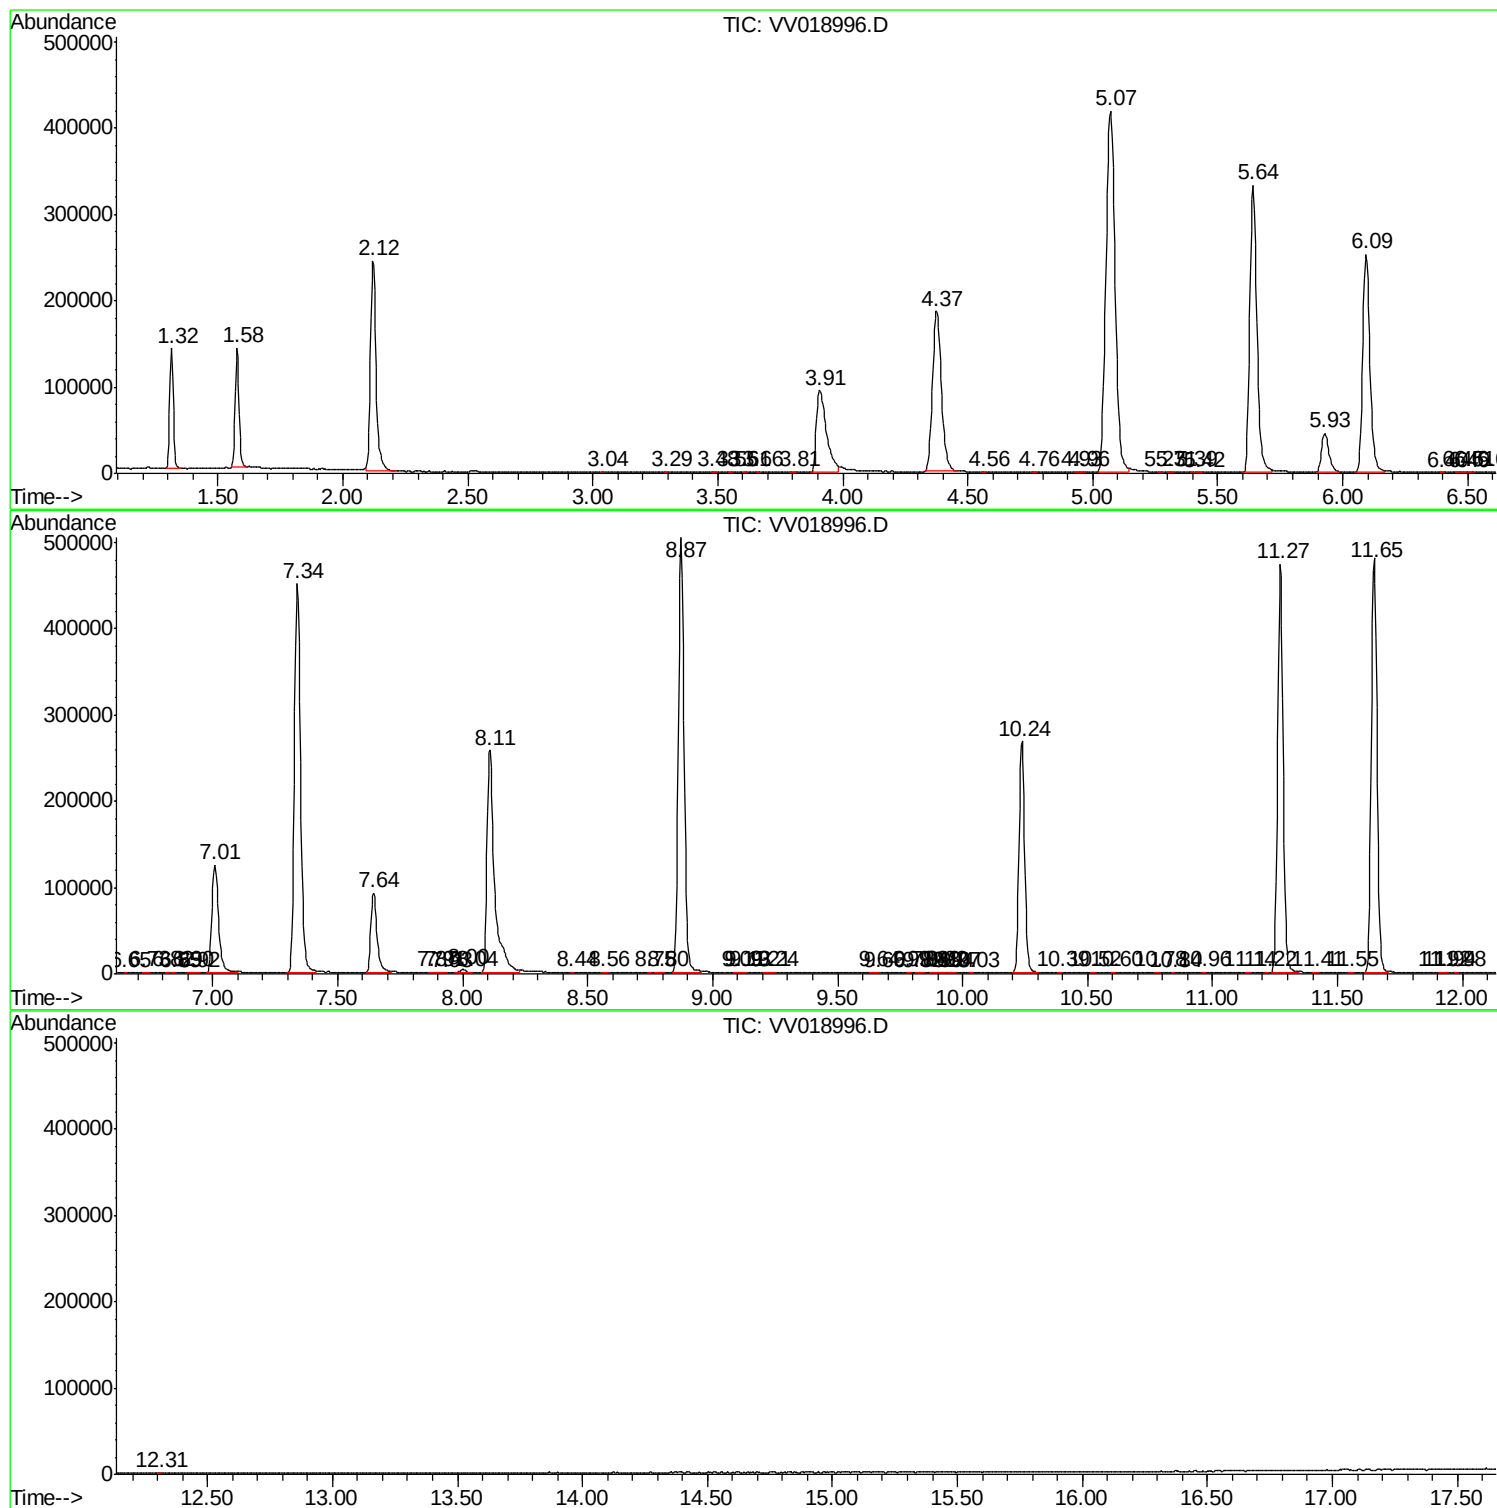

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018996.D
Acq On : 20 Oct 2020 03:55
Operator : SY/MD
Sample : L4430-10 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018996.D
Acq On : 20 Oct 2020 03:55
Operator : SY/MD
Sample : L4430-10 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc