


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV101920\
Data File : VV018960.D
Acq On : 19 Oct 2020 09:54
Operator : SY/MD
Sample : BFB77
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB77

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis
Last Update : Tue Oct 20 03:20:26 2020

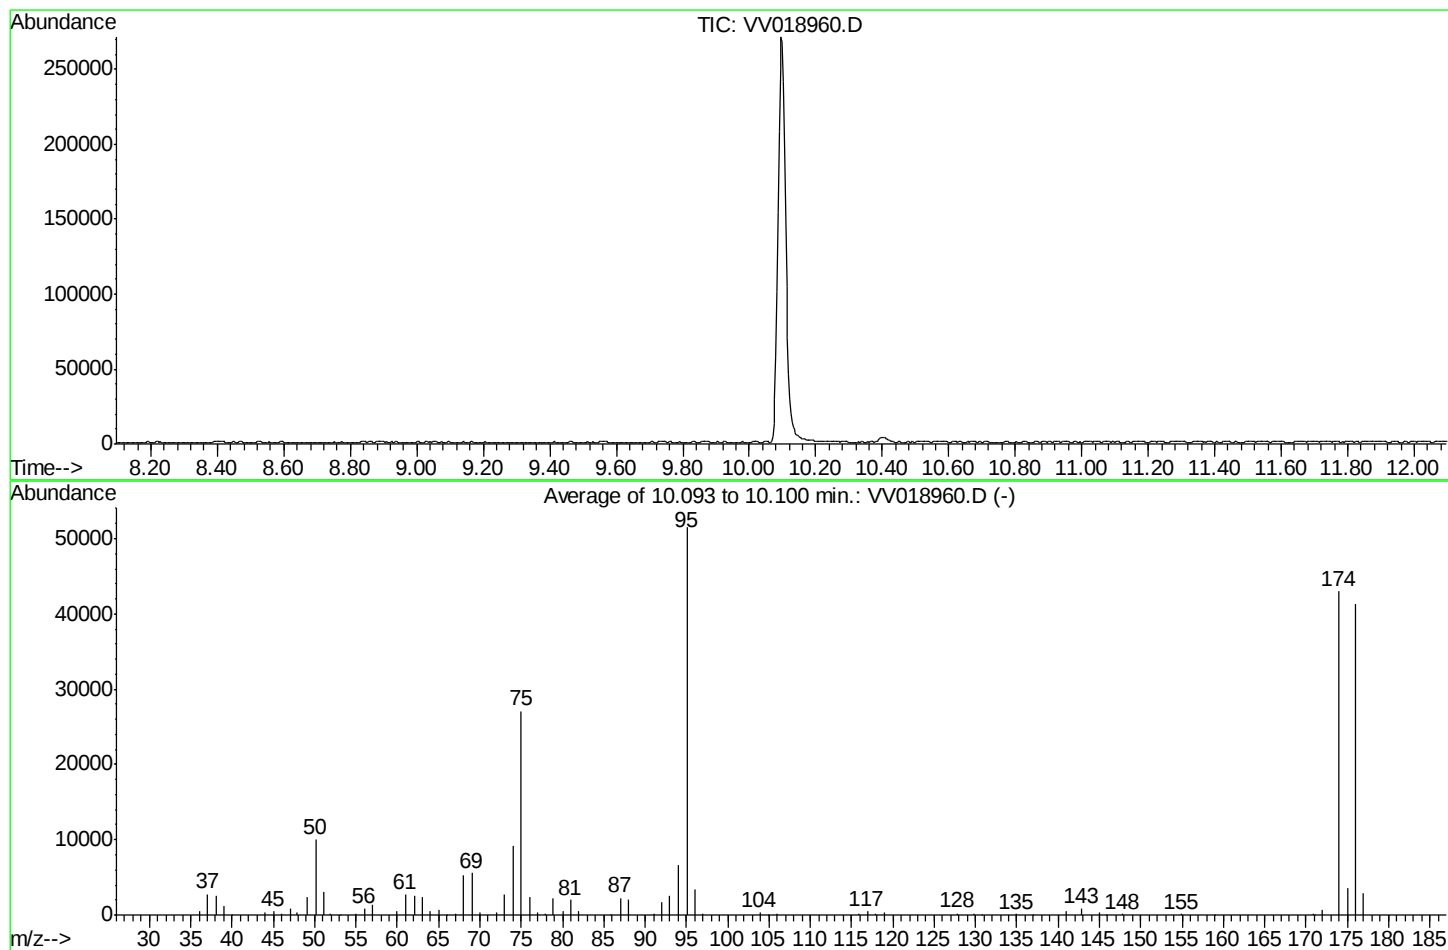

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	10008	PASS
75	95	30	80	52.5	27048	PASS
95	95	100	100	100.0	51501	PASS
96	95	5	9	6.5	3361	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.5	43010	PASS
175	174	5	9	8.3	3586	PASS
176	174	95	101	96.0	41280	PASS
177	176	5	9	6.9	2849	PASS

m/z	Abundance
36.00	536.0
37.00	2742.0
38.00	2404.0
39.00	1172.0
40.00	301.0
44.00	1338.0
45.00	476.0
46.10	106.0
47.00	865.0
47.90	359.0
49.10	2382.0
50.10	9469.0
51.10	2973.0
52.00	177.0
53.10	135.0
55.10	169.0
56.10	713.0
57.10	1135.0
59.90	630.0
61.00	2650.0
62.10	2342.0
63.00	2182.0
63.90	425.0
65.00	614.0
67.00	191.0
68.00	5323.0
69.00	5314.0
70.00	399.0
72.00	345.0
73.00	2455.0
74.00	8611.0
75.00	25848.0
76.00	2279.0
77.00	294.0
78.00	208.0
78.90	2082.0
80.00	536.0
80.90	1953.0
81.90	502.0
85.90	123.0
87.00	2172.0
88.00	2074.0
91.00	215.0
92.00	1516.0
93.00	2459.0
94.00	6556.0
95.10	48832.0
96.00	3129.0
97.00	174.0
103.90	221.0
105.90	274.0
116.00	200.0
116.90	460.0
117.90	170.0
118.90	359.0
127.90	193.0
129.80	200.0
135.00	121.0
140.90	495.0
142.90	726.0
144.90	312.0
147.80	144.0
154.90	158.0
170.90	190.0
172.00	658.0
174.00	40400.0
175.00	3422.0
176.00	38944.0
177.00	2691.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.00	604.0
37.10	2868.0
38.00	2591.0
39.00	1162.0
40.00	297.0
44.00	1380.0
45.00	506.0
46.00	110.0
47.00	833.0
47.90	359.0
49.10	2476.0
50.10	10221.0
51.10	3101.0
52.00	161.0
53.20	104.0
55.00	205.0
56.00	801.0
57.00	1294.0
59.90	595.0
61.00	2837.0
62.10	2584.0
63.00	2424.0
63.90	458.0
65.00	671.0
65.90	110.0
67.00	181.0
68.00	5486.0
69.00	5758.0
70.10	400.0
72.00	345.0
73.00	2703.0
74.00	9425.0
75.00	27944.0
76.00	2435.0
77.00	284.0
77.90	256.0
78.90	2280.0
80.00	602.0
80.90	2048.0
81.90	518.0
85.80	115.0
87.00	2260.0
88.00	2077.0
91.00	220.0
92.00	1702.0
93.00	2708.0
94.00	6983.0
95.10	53376.0
96.00	3436.0
97.00	172.0
103.90	287.0
104.90	108.0
106.00	267.0
115.90	193.0
116.90	500.0
117.90	199.0
118.90	360.0
127.80	231.0
129.80	209.0
130.80	103.0
135.00	161.0
136.90	102.0
140.90	613.0
142.90	823.0
144.90	334.0
145.90	101.0
147.80	147.0
155.00	133.0
170.90	163.0
172.00	742.0
174.00	44272.0
175.00	3716.0
176.00	42480.0
177.00	2969.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.00	618.0
37.10	2655.0
38.10	2538.0
39.00	1072.0
39.90	228.0
44.00	1427.0
45.00	492.0
45.90	106.0
47.00	727.0
47.90	350.0
49.10	2278.0
50.10	10335.0
51.10	3045.0
51.90	163.0
54.90	244.0
56.00	850.0
57.00	1431.0
59.90	541.0
61.00	2675.0
62.00	2629.0
63.00	2411.0
63.90	459.0
65.00	694.0
65.90	132.0
67.00	195.0
68.00	5171.0
69.00	5696.0
70.10	368.0
72.00	360.0
73.00	2823.0
74.00	9380.0
75.00	27352.0
76.10	2375.0
77.00	300.0
77.90	269.0
78.90	2189.0
80.00	609.0
81.00	1958.0
81.90	519.0
87.00	2206.0
88.00	1972.0
91.00	207.0
92.00	1790.0
93.00	2651.0
94.00	6551.0
95.10	52296.0
96.00	3518.0
97.00	135.0
103.90	301.0
104.90	141.0
105.90	241.0
115.80	215.0
116.90	471.0
117.80	203.0
118.90	374.0
127.80	238.0
129.90	224.0
130.80	122.0
135.00	188.0
136.90	114.0
140.90	611.0
142.90	822.0
145.00	320.0
145.80	101.0
147.80	130.0
154.90	103.0
159.00	106.0
171.10	146.0
172.00	756.0
174.00	44360.0
175.00	3621.0
176.00	42416.0
177.00	2887.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

Scan 2790 (10.061 min): VV018960.D
BFB77

m/z	Abundance
39.90	233.0
44.00	1038.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77