

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101921\
 Data File : VV022914.D
 Acq On : 19 Oct 2021 13:19
 Operator : SY/MD
 Sample : M4214-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 20 08:18:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101921.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 20 08:16:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	11004	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	10609	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	5951	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	9222	0.551	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	110.000%
4) 1,2-Dichloroethane-d4	5.042	65	4566	0.496	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
7) 1,2-Dichloropropane-d6	6.068	67	5840	0.497	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	100.000%
8) Toluene-d8	7.317	98	14803	0.487	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	3801	0.505	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	102.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.426	75	20	0.017	ug/L	Qvalue # 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101921\
Data File : VV022914.D
Acq On : 19 Oct 2021 13:19
Operator : SY/MD
Sample : M4214-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 20 08:18:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101921.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 20 08:16:40 2021
Response via : Initial Calibration

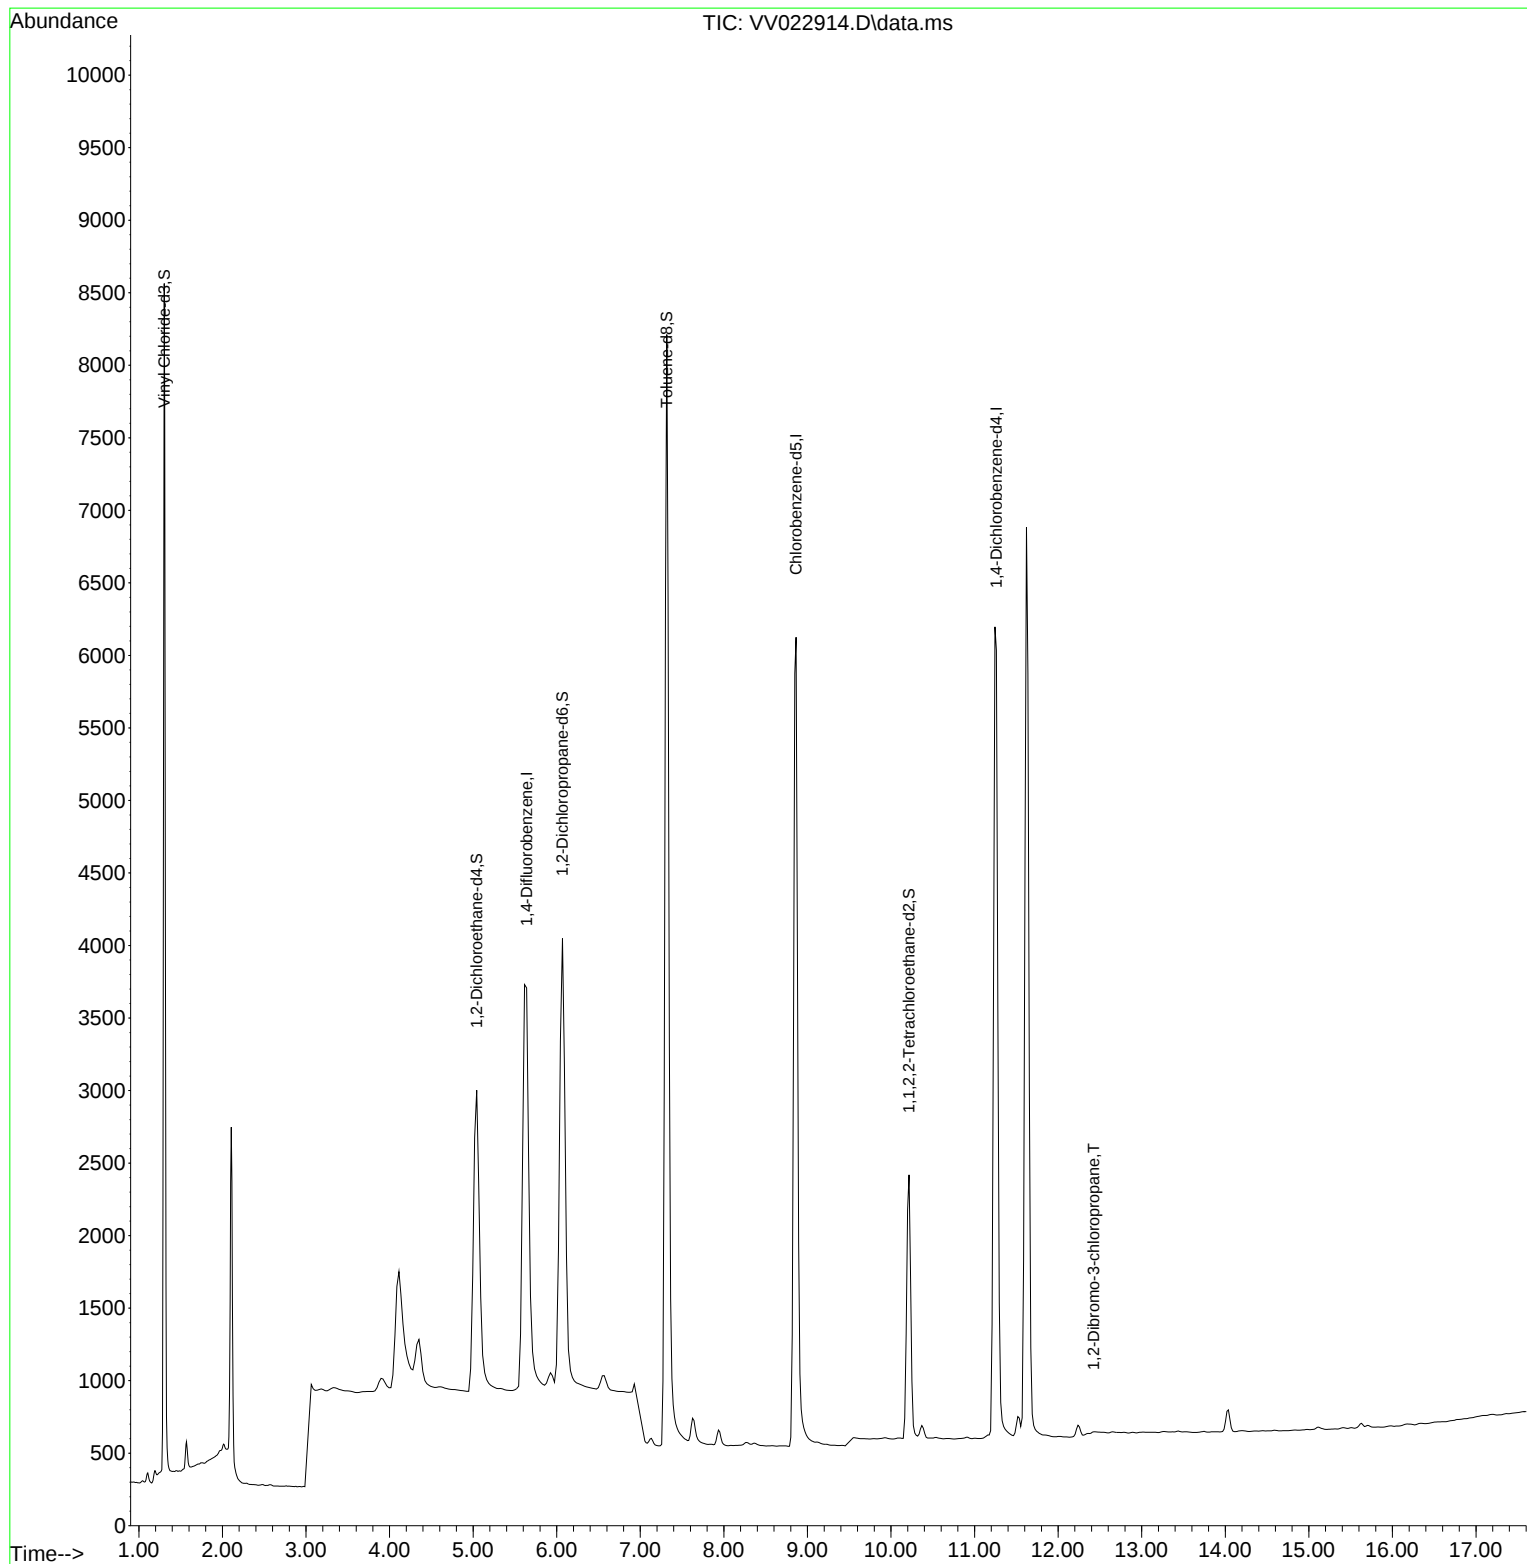

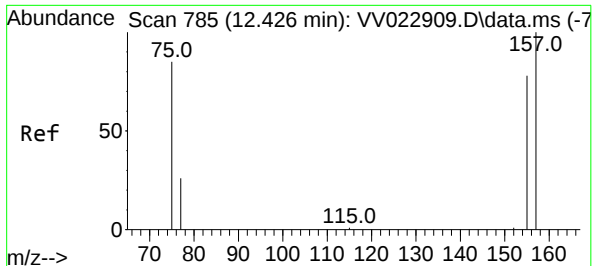

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.017 ug/L
 RT: 12.426 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV022914.D
 Acq: 19 Oct 2021 13:19

Instrument :
 MSVOA_V
 ClientSampleId :

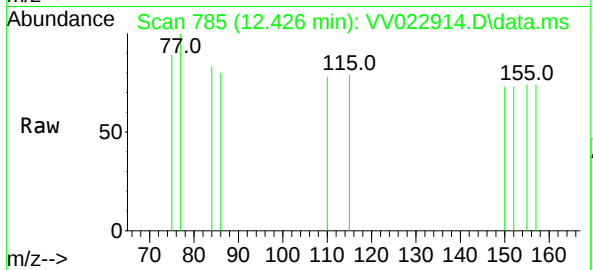

Tgt Ion: 75 Resp: 20
 Ion Ratio Lower Upper
 75 100
 157 83.3 86.7 130.1#
 155 83.3 71.9 107.9

