

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101921\
 Data File : VV022915.D
 Acq On : 19 Oct 2021 13:43
 Operator : SY/MD
 Sample : M4214-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 20 08:18:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101921.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 20 08:16:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	10613	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	10576	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	5758	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	8690	0.538	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	108.000%
4) 1,2-Dichloroethane-d4	5.042	65	4861	0.547	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	110.000%
7) 1,2-Dichloropropane-d6	6.068	67	6276	0.536	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.000%
8) Toluene-d8	7.317	98	15025	0.496	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
10) 1,1,2,2-Tetrachloroeth...	10.215	84	4217	0.562	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	112.000%
Target Compounds						
6) Trichloroethene	5.925	95	560	0.052	ug/L	91
13) 1,2-Dibromo-3-chloropr...	12.238	75	199	0.174	ug/L #	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101921\
Data File : VV022915.D
Acq On : 19 Oct 2021 13:43
Operator : SY/MD
Sample : M4214-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 20 08:18:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101921.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 20 08:16:40 2021
Response via : Initial Calibration

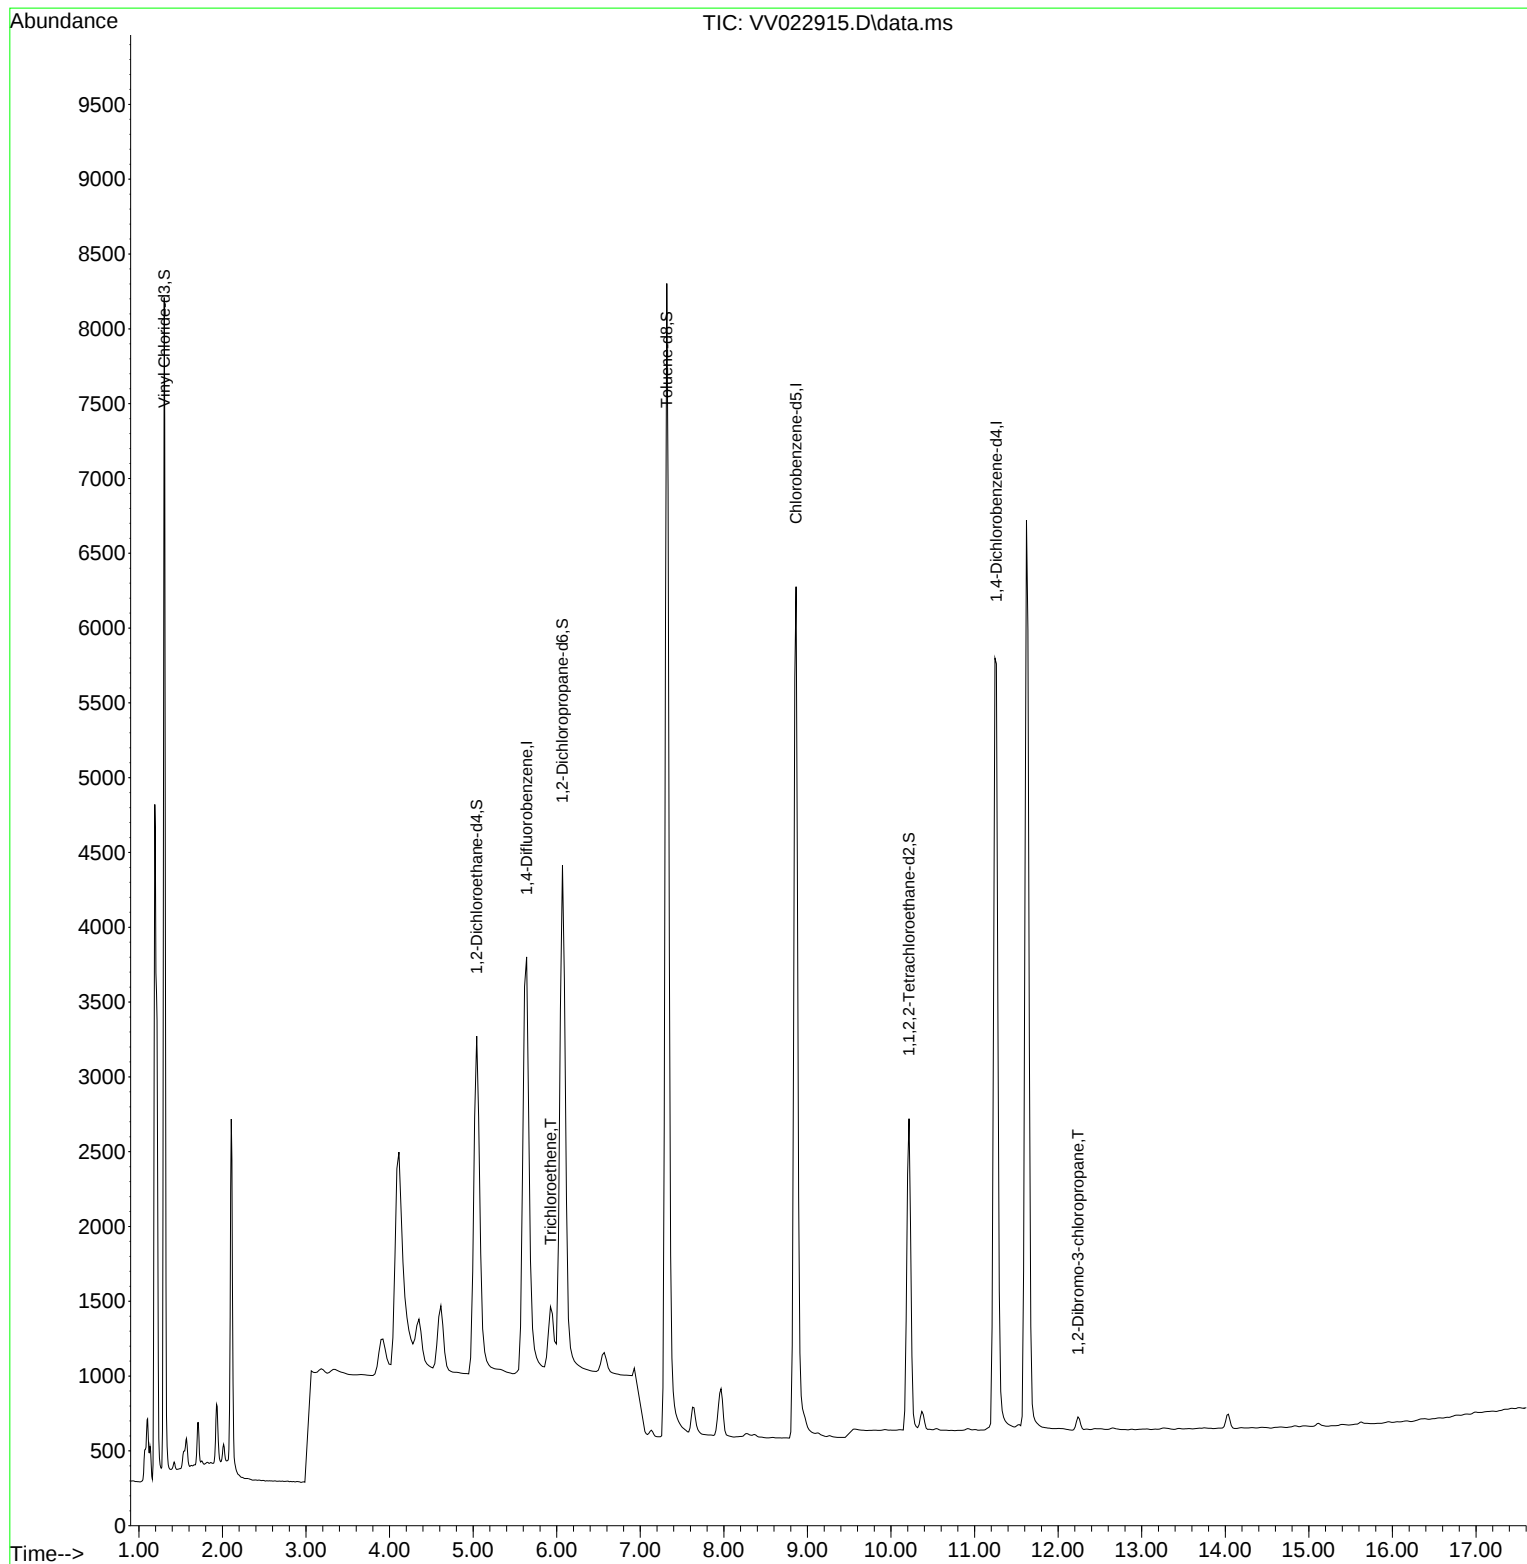

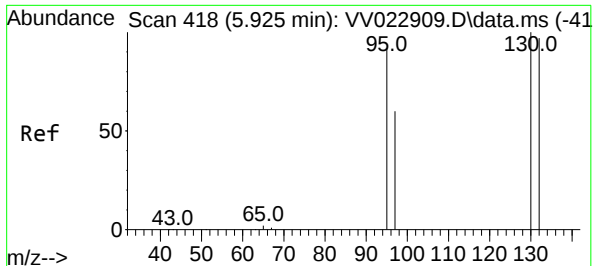




#6
Trichloroethene
Concen: 0.052 ug/L
RT: 5.925 min Scan# 418
Delta R.T. -0.000 min
Lab File: VV022915.D
Acq: 19 Oct 2021 13:43

Instrument :
MSVOA_V
ClientSampled :

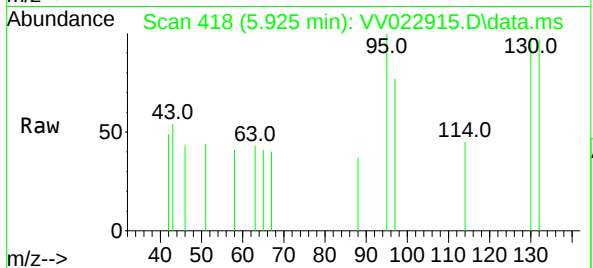


Tgt Ion: 95 Resp: 560

Ion	Ratio	Lower	Upper
95	100		
97	76.8	47.1	87.5
132	96.7	73.0	135.6
130	98.3	75.5	140.3

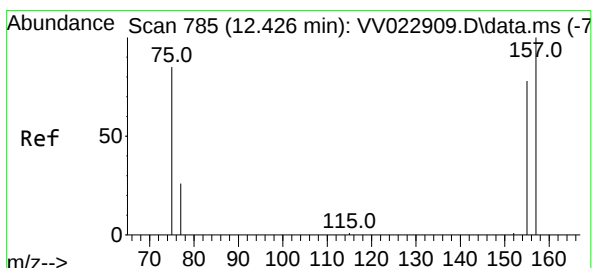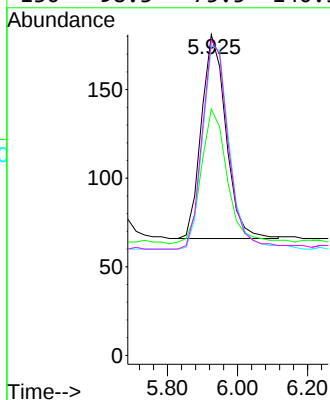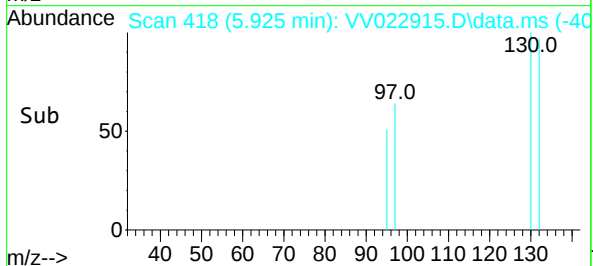

#13
1,2-Dibromo-3-chloropropane
Concen: 0.174 ug/L
RT: 12.238 min Scan# 774
Delta R.T. -0.189 min
Lab File: VV022915.D
Acq: 19 Oct 2021 13:43

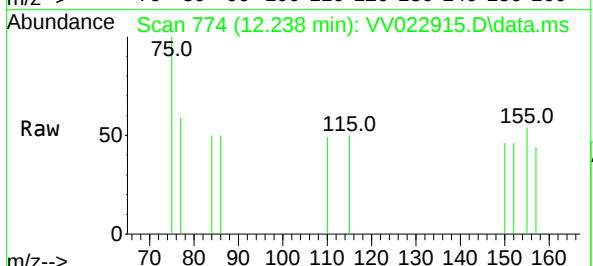

Tgt Ion: 75 Resp: 199

Ion	Ratio	Lower	Upper
75	100		
157	43.6	86.7	130.1#
155	54.1	71.9	107.9#

