

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101921\
 Data File : VV022920.D
 Acq On : 19 Oct 2021 15:42
 Operator : SY/MD
 Sample : M4214-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 20 08:18:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101921.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 20 08:16:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	10649	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	10582	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	5647	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	9021	0.557	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 112.000%			
4) 1,2-Dichloroethane-d4	5.042	65	4952	0.556	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 112.000%			
7) 1,2-Dichloropropane-d6	6.068	67	6463	0.551	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 110.000%			
8) Toluene-d8	7.317	98	14707	0.485	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 96.000%			
10) 1,1,2,2-Tetrachloroeth...	10.216	84	4364	0.581	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 116.000%			
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.427	75	10	0.009	ug/L	Qvalue # 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101921\
Data File : VV022920.D
Acq On : 19 Oct 2021 15:42
Operator : SY/MD
Sample : M4214-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 20 08:18:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101921.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 20 08:16:40 2021
Response via : Initial Calibration

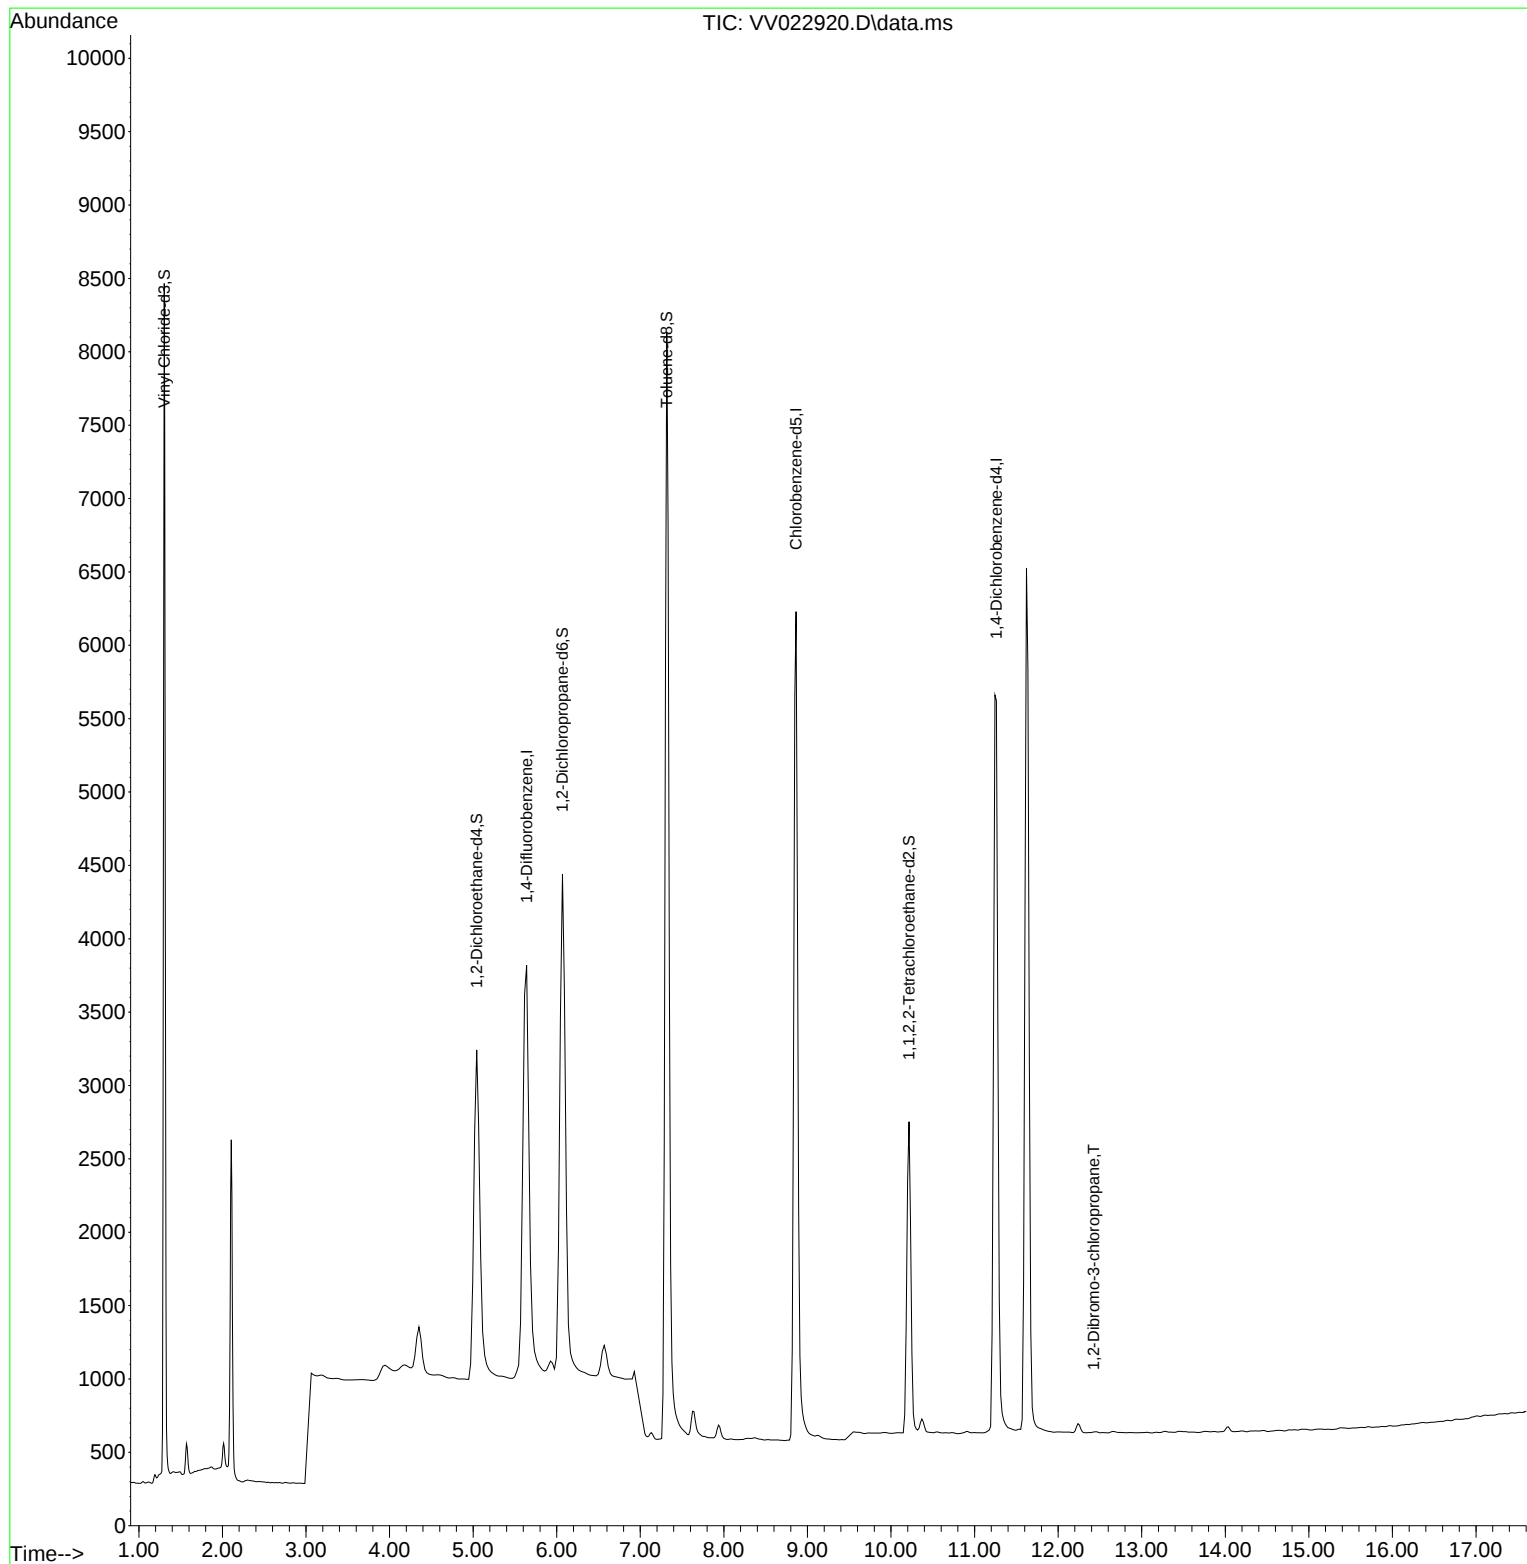

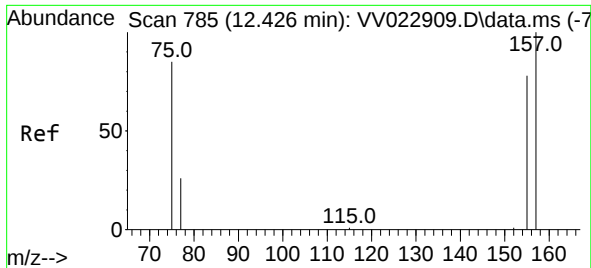

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.009 ug/L
 RT: 12.427 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV022920.D
 Acq: 19 Oct 2021 15:42

Instrument :
 MSVOA_V
 ClientSampleId :

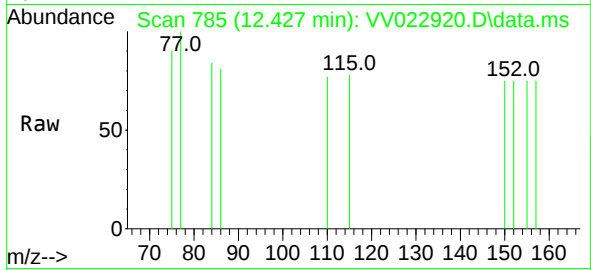

Tgt Ion: 75 Resp: 10
 Ion Ratio Lower Upper
 75 100
 157 83.1 86.7 130.1#
 155 83.1 71.9 107.9

