

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101921\
 Data File : VV022916.D
 Acq On : 19 Oct 2021 14:08
 Operator : SY/MD
 Sample : M4214-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JDGG7

Quant Time: Oct 20 08:18:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101921.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 20 08:16:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	10599	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	10531	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	5776	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	8732	0.542	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	108.000%
4) 1,2-Dichloroethane-d4	5.042	65	4760	0.537	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
7) 1,2-Dichloropropane-d6	6.068	67	6182	0.530	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	106.000%
8) Toluene-d8	7.317	98	14481	0.480	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	96.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	4222	0.565	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	114.000%
Target Compounds						
6) Trichloroethene	5.925	95	570	0.054	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101921\
Data File : VV022916.D
Acq On : 19 Oct 2021 14:08
Operator : SY/MD
Sample : M4214-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGG7


Quant Time: Oct 20 08:18:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101921.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 20 08:16:40 2021
Response via : Initial Calibration

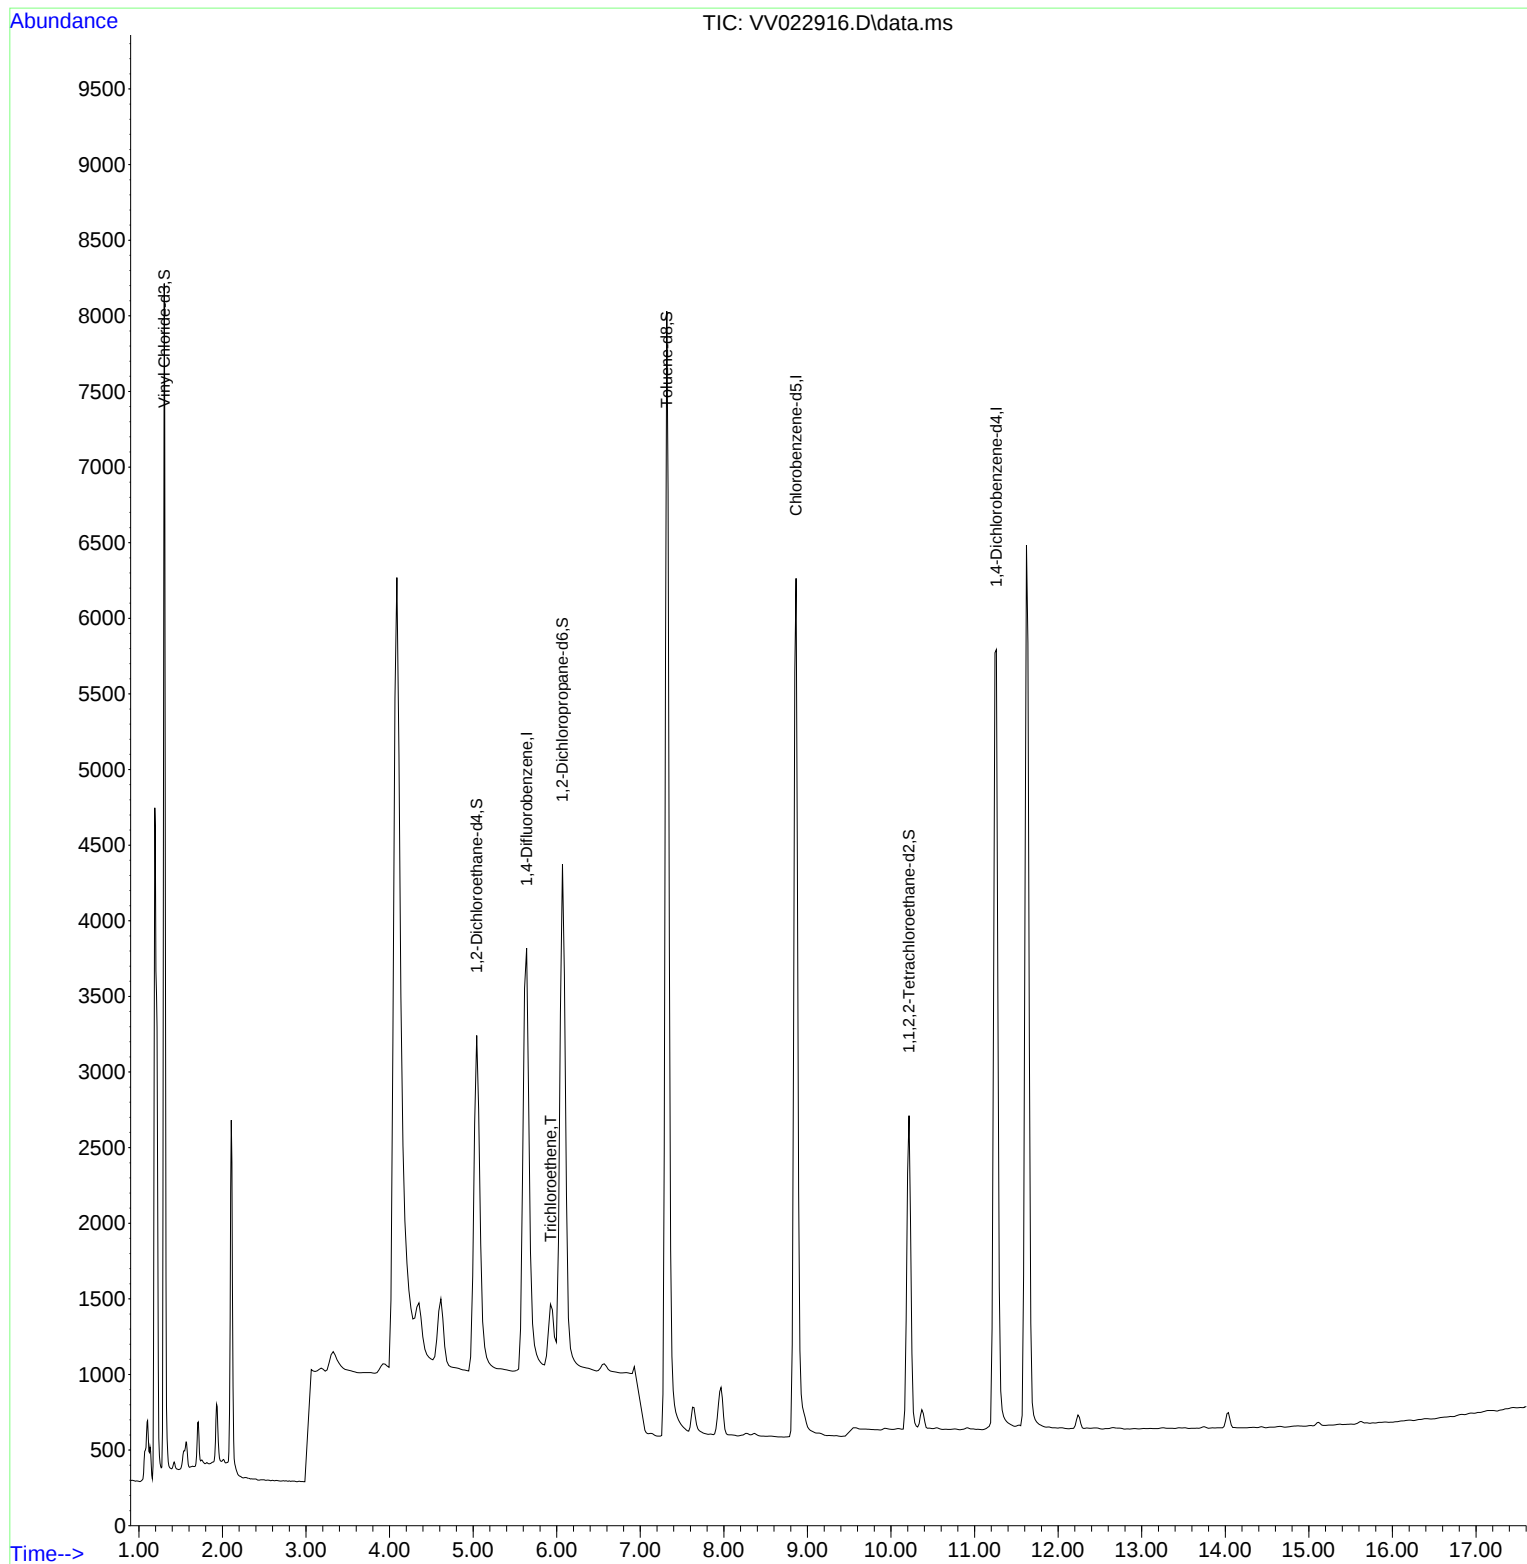

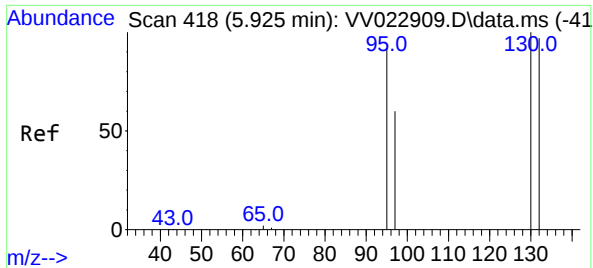

#6
Trichloroethene
Concen: 0.054 ug/L
RT: 5.925 min Scan# 418
Delta R.T. 0.000 min
Lab File: VV022916.D
Acq: 19 Oct 2021 14:08

Instrument :
MSVOA_V
ClientSampleId :
JDGG7

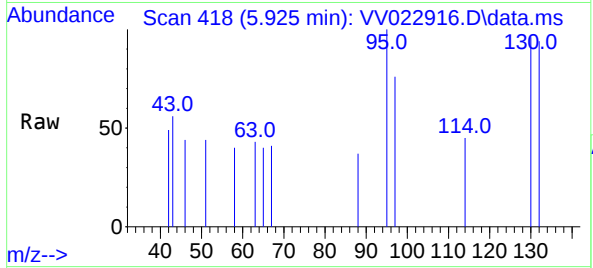

Tgt Ion: 95 Resp: 570

Ion	Ratio	Lower	Upper
95	100		
97	75.8	47.1	87.5
132	94.0	73.0	135.6
130	96.2	75.5	140.3

