
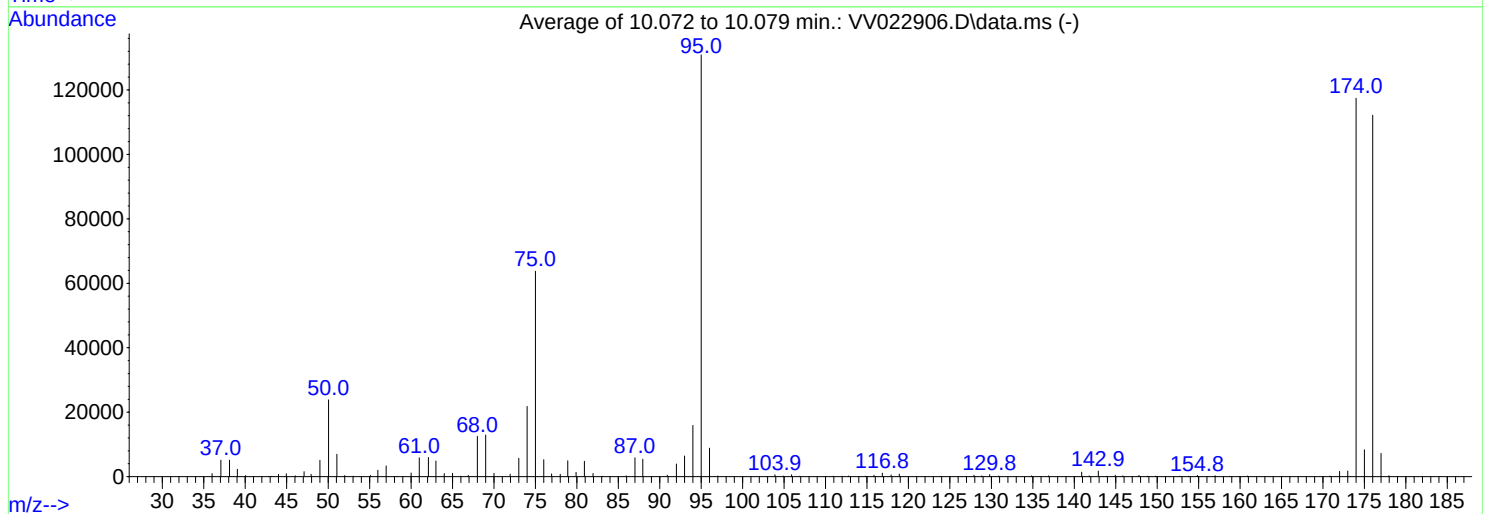


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101921\
 Data File : VV022906.D
 Acq On : 19 Oct 2021 09:30
 Operator : SY/MD
 Sample : BFB205
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB205

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101921.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Oct 20 08:16:40 2021

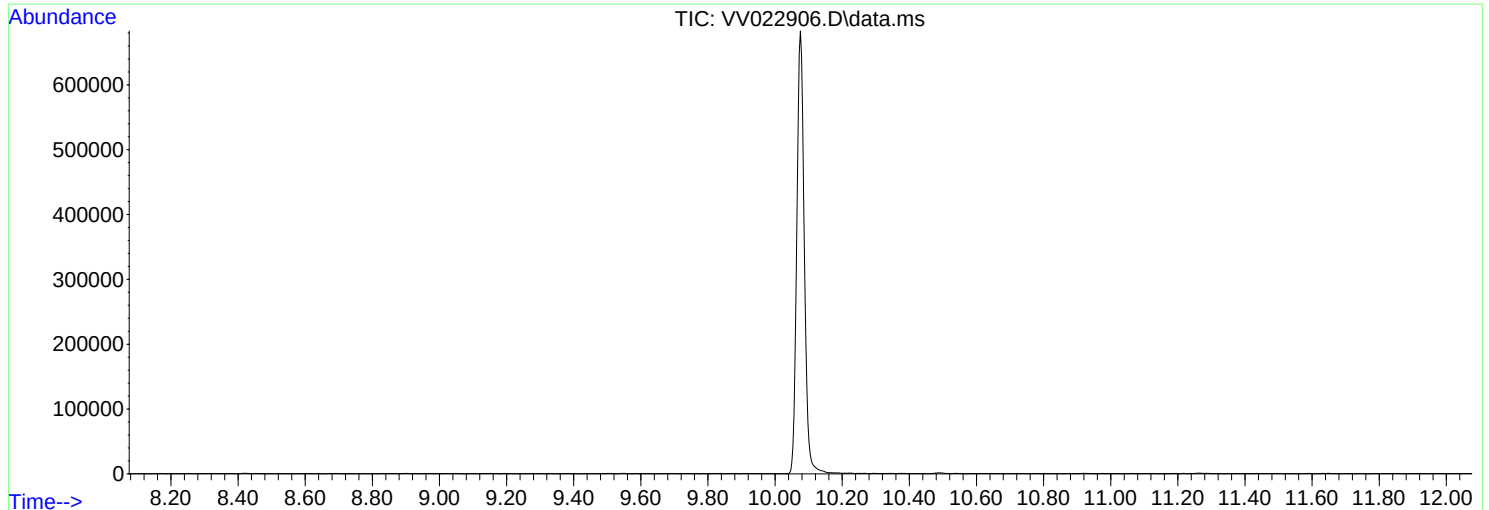

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	23827	PASS
75	95	30	80	48.7	63757	PASS
95	95	100	100	100.0	130899	PASS
96	95	5	9	6.7	8829	PASS
173	174	0.00	2	1.5	1721	PASS
174	95	50	120	89.7	117413	PASS
175	174	5	9	7.1	8335	PASS
176	174	95	101	95.5	112187	PASS
177	176	5	9	6.4	7204	PASS

m/z	Abundance
36.00	980.0
37.00	5222.0
38.10	5256.0
39.00	2406.0
40.00	358.0
43.20	132.0
44.00	902.0
45.00	1042.0
46.00	261.0
47.10	1612.0
48.00	758.0
49.00	5301.0
50.00	24840.0
51.10	7166.0
52.00	375.0
53.10	161.0
55.10	326.0
56.00	2065.0
57.00	3441.0
58.30	156.0
60.00	1209.0
61.00	6022.0
62.10	6195.0
63.00	5025.0
64.00	986.0
65.00	1084.0
66.00	164.0
66.90	464.0
68.00	12993.0
69.00	13398.0
70.00	1104.0
71.90	850.0
73.00	5872.0
74.00	22584.0
75.00	65944.0
76.00	5335.0
76.90	898.0
78.00	782.0
78.90	5133.0
79.90	1344.0
80.90	5005.0
82.00	1039.0
83.10	166.0
85.90	276.0
87.00	6057.0
88.00	5616.0
90.90	506.0
92.00	4115.0
93.00	6716.0
94.00	16536.0
95.00	135424.0
96.00	9102.0
97.00	208.0
102.90	105.0
103.90	600.0
104.90	231.0
105.90	599.0
106.90	149.0
109.90	107.0
110.90	165.0
112.00	147.0
112.70	181.0
114.80	179.0
115.80	441.0
116.90	1122.0
117.90	580.0
118.90	843.0
123.80	121.0
127.90	429.0
128.80	267.0
129.80	707.0
130.90	193.0
134.80	234.0
136.90	296.0
140.10	108.0
140.90	1438.0
141.80	270.0
142.90	1783.0
143.90	147.0
145.00	442.0
145.80	275.0
146.90	110.0
147.80	423.0
148.80	176.0
149.80	146.0
152.80	125.0
153.80	140.0
154.80	399.0
157.00	310.0
158.70	120.0
159.00	127.0
160.90	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

170.90	208.0
172.00	1732.0
173.00	1769.0
174.00	121528.0
175.00	8666.0
176.00	116040.0
177.00	7430.0
177.90	338.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

Scan 2796 (10.030 min): VV022906.D\data.ms
BFB205

m/z	Abundance
39.80	113.0
44.00	185.0
44.80	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	986.0
37.00	5111.0
38.10	5012.0
39.00	2153.0
40.00	345.0
42.80	124.0
44.00	915.0
45.00	1009.0
46.10	209.0
47.10	1539.0
48.00	760.0
49.00	5135.0
50.10	23864.0
51.00	6942.0
52.00	388.0
53.10	185.0
55.00	362.0
56.00	2035.0
57.00	3562.0
58.00	161.0
60.00	1131.0
61.00	5783.0
62.10	6020.0
63.00	4898.0
64.00	989.0
65.00	1019.0
66.00	179.0
66.90	427.0
68.00	12516.0
69.00	12759.0
70.00	978.0
72.00	787.0
73.00	5745.0
74.00	21736.0
75.00	63816.0
76.00	5534.0
76.90	895.0
78.00	787.0
78.90	4838.0
79.90	1444.0
80.90	4765.0
81.90	1070.0
83.10	161.0
86.00	268.0
87.00	6082.0
87.90	5345.0
90.90	447.0
92.00	3952.0
93.00	6417.0
94.00	15812.0
95.00	129536.0
96.00	8806.0
97.00	219.0
102.90	131.0
103.90	548.0
104.90	221.0
105.90	566.0
106.90	146.0
110.90	144.0
112.00	138.0
112.80	180.0
114.80	142.0
115.80	491.0
116.90	1069.0
117.90	559.0
118.90	808.0
123.80	105.0
127.90	412.0
128.80	259.0
129.80	605.0
131.00	187.0
134.80	267.0
136.90	242.0
140.90	1489.0
141.80	227.0
142.90	1686.0
144.00	170.0
145.00	454.0
145.90	282.0
147.80	329.0
148.80	122.0
149.80	136.0
152.80	137.0
154.80	379.0
157.00	282.0
158.70	143.0
160.90	179.0
170.80	230.0
172.00	1719.0
173.00	1826.0
174.00	114072.0
175.00	8059.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

176.00	108200.0
177.00	6938.0
178.00	275.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	950.0
37.10	5023.0
38.10	5062.0
39.10	2333.0
40.10	313.0
43.20	125.0
44.00	825.0
45.00	983.0
46.00	285.0
47.10	1440.0
47.90	706.0
49.00	4795.0
50.10	22776.0
51.10	6837.0
52.00	318.0
53.00	143.0
55.20	316.0
56.00	1850.0
57.00	3023.0
58.30	149.0
60.00	1170.0
61.00	5811.0
62.10	5750.0
63.00	4749.0
64.00	873.0
65.00	1038.0
66.00	123.0
66.90	377.0
68.00	12010.0
69.00	12634.0
70.00	1035.0
72.00	765.0
73.00	5465.0
74.00	21144.0
75.00	61512.0
76.00	4921.0
77.00	796.0
78.00	664.0
78.90	4843.0
79.90	1178.0
80.90	4566.0
82.00	932.0
83.00	172.0
85.90	271.0
87.00	5512.0
88.00	5296.0
90.90	455.0
92.00	3672.0
93.00	6153.0
94.00	15302.0
95.00	127736.0
96.00	8579.0
97.00	185.0
103.90	619.0
104.90	204.0
105.90	581.0
106.90	143.0
110.00	130.0
110.90	192.0
112.00	110.0
112.70	170.0
114.80	177.0
115.90	422.0
116.80	1057.0
117.90	518.0
118.90	780.0
123.80	124.0
127.90	449.0
128.90	245.0
129.80	655.0
130.80	199.0
134.90	236.0
136.90	283.0
140.90	1295.0
141.80	263.0
142.90	1704.0
143.90	123.0
144.80	400.0
145.80	247.0
147.00	123.0
147.80	509.0
148.80	168.0
149.80	160.0
152.60	124.0
153.80	181.0
154.90	357.0
157.00	298.0
159.00	131.0
160.90	196.0
170.90	204.0
172.00	1558.0
173.00	1568.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

174.00	116640.0
175.00	8279.0
176.00	112320.0
177.00	7244.0
177.90	298.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205