

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032493.D
 Acq On : 19 Oct 2023 13:40
 Operator : SY/MD
 Sample : 04944-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 20 06:22:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 20 06:17:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	92153	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	103501	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	47392	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	36035	4.808	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.200%
7) Chloroethane-d5	1.532	69	31995	5.259	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.200%
11) 1,1-Dichloroethene-d2	2.060	65	13724	4.342	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.800%
20) 2-Butanone-d5	3.809	46	84825	44.741	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.480%
24) Chloroform-d	4.256	84	60023	4.540	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.800%
26) 1,2-Dichloroethane-d4	4.947	65	31467	5.025	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	4.963	84	121996	4.006	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.200%
36) 1,2-Dichloropropane-d6	5.992	67	40657	4.029	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.600%
41) Toluene-d8	7.246	98	106855	3.837	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.800%
43) trans-1,3-Dichloroprop...	7.561	79	14526	4.063	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.200%
46) 2-Hexanone-d5	8.031	63	72790	43.267	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.540%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	32357	4.585	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.600%
66) 1,2-Dichlorobenzene-d4	11.564	152	40398	4.594	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.800%
Target Compounds						
61) 1,2,3-Trichloropropane	11.188	75	6266	1.242	ug/L	Qvalue # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032493.D
Acq On : 19 Oct 2023 13:40
Operator : SY/MD
Sample : 04944-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 20 06:22:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 20 06:17:42 2023
Response via : Initial Calibration

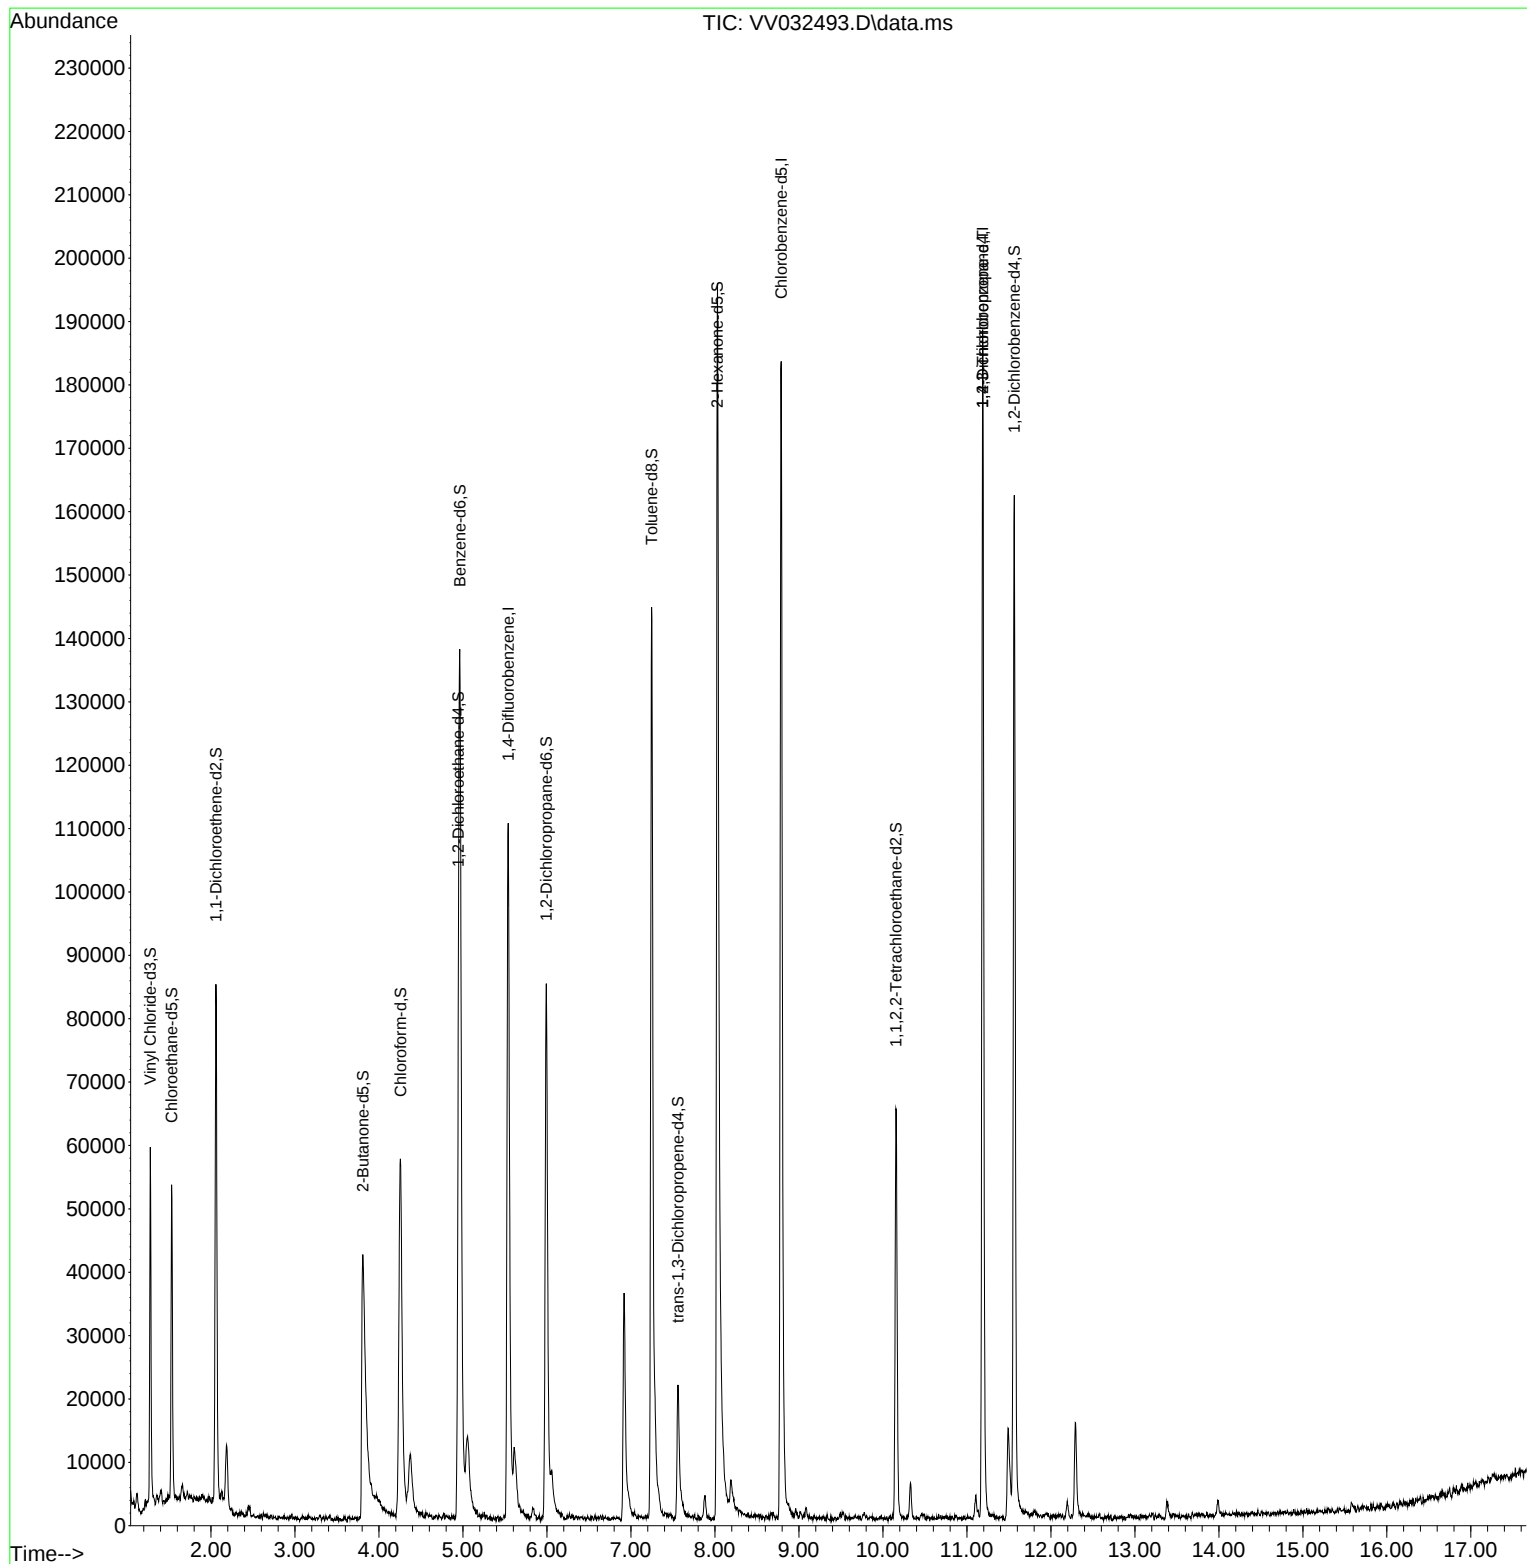

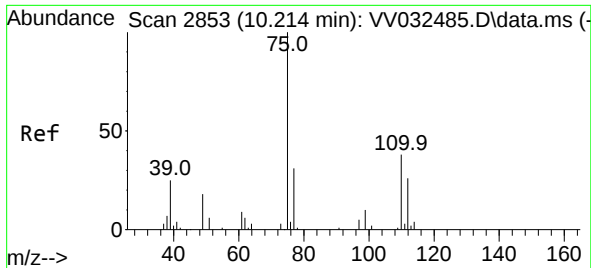

#61
 1,2,3-Trichloropropane
 Concen: 1.242 ug/L
 RT: 11.188 min Scan# 31
 Delta R.T. 0.974 min
 Lab File: VV032493.D
 Acq: 19 Oct 2023 13:40

Instrument :
 MSVOA_V
 ClientSampleId :

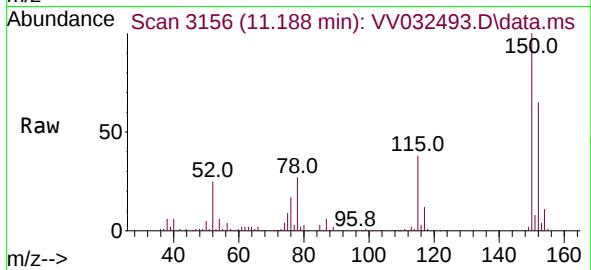

Tgt Ion: 75 Resp: 6266
 Ion Ratio Lower Upper
 75 100
 77 33.1 26.2 39.2
 110 3.6 30.6 46.0#

