




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV101923\  
 Data File : VV032495.D  
 Acq On : 19 Oct 2023 14:29  
 Operator : SY/MD  
 Sample : 04918-15  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AH2

Manual IntegrationsAPPROVED

Quant Time: Oct 20 06:22:34 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Oct 20 06:17:42 2023  
 Response via : Initial Calibration

Reviewed By : John Carlone 10/20/2023  
 Supervised By : Mahesh Dadoda 10/24/2023

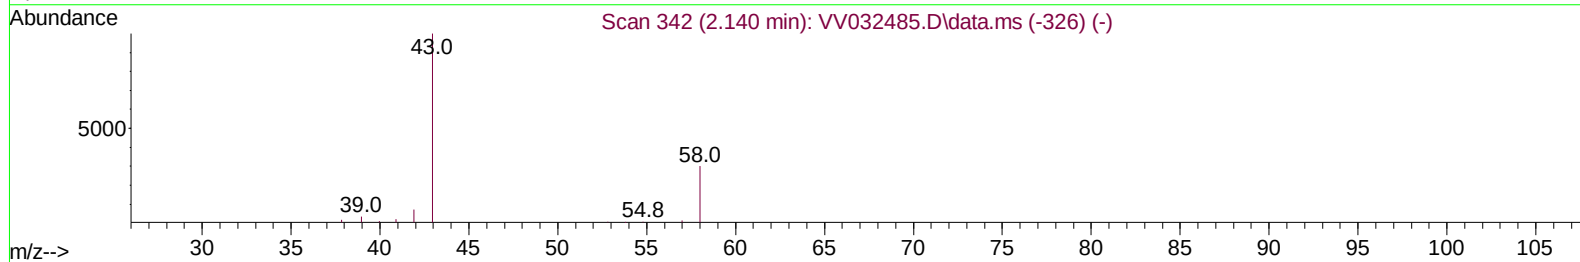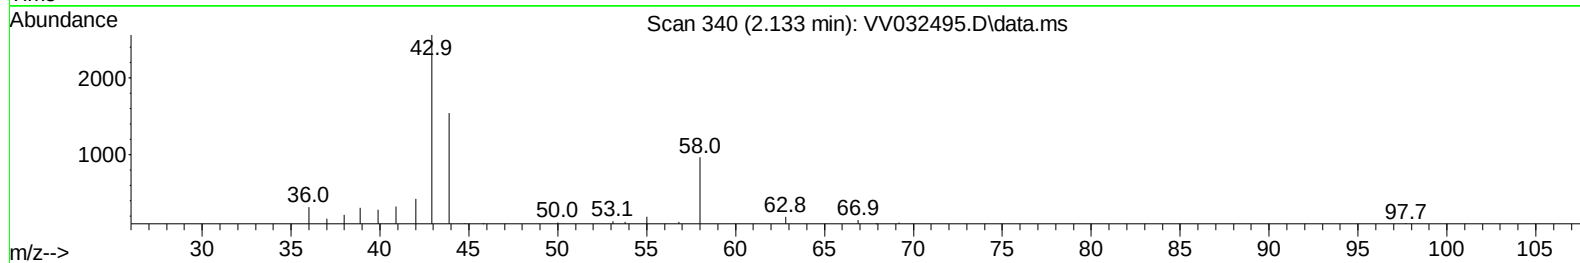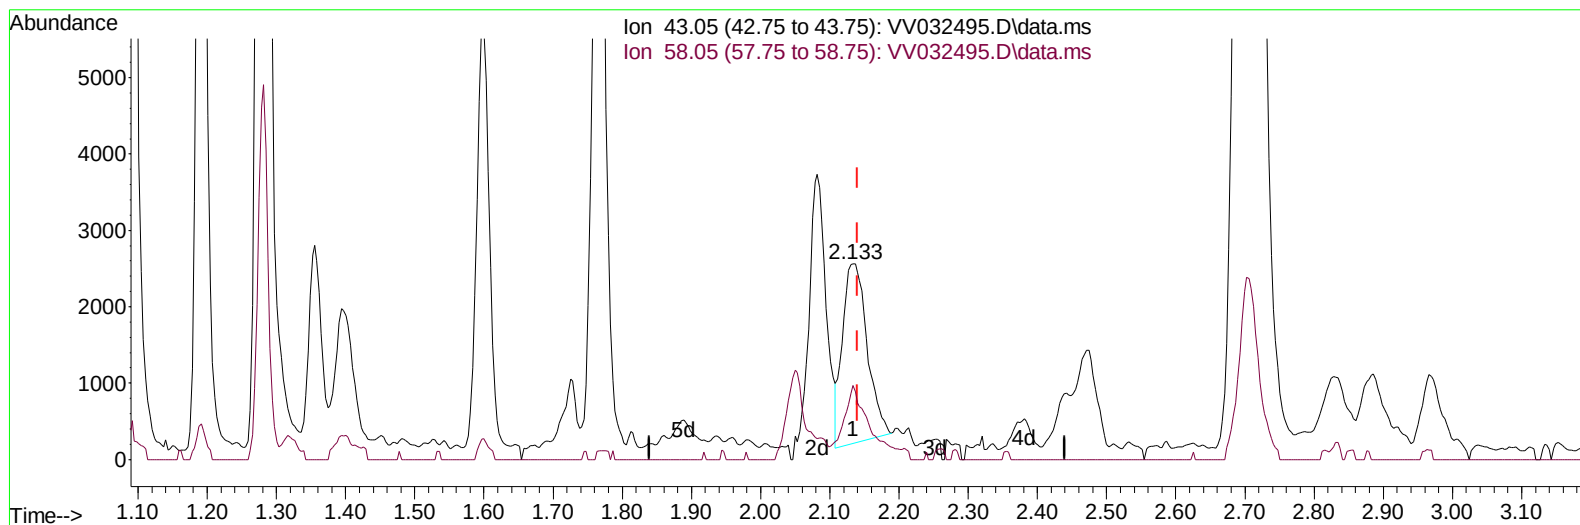

TIC: VV032495.D\data.ms

(13) Acetone (T)

2.133min (-0.006) 3.66 ug/L

response 5862

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 33.00  | 32.79  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV101923\  
 Data File : VV032495.D  
 Acq On : 19 Oct 2023 14:29  
 Operator : SY/MD  
 Sample : 04918-15  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AH2

Manual IntegrationsAPPROVED

Quant Time: Oct 20 06:22:34 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Oct 20 06:17:42 2023  
 Response via : Initial Calibration

Reviewed By :John Carlone 10/20/2023  
 Supervised By :Mahesh Dadoda 10/24/2023

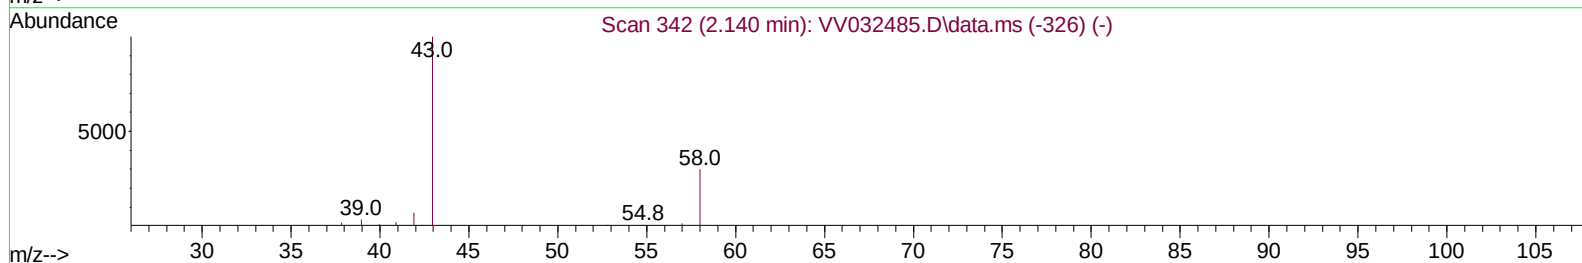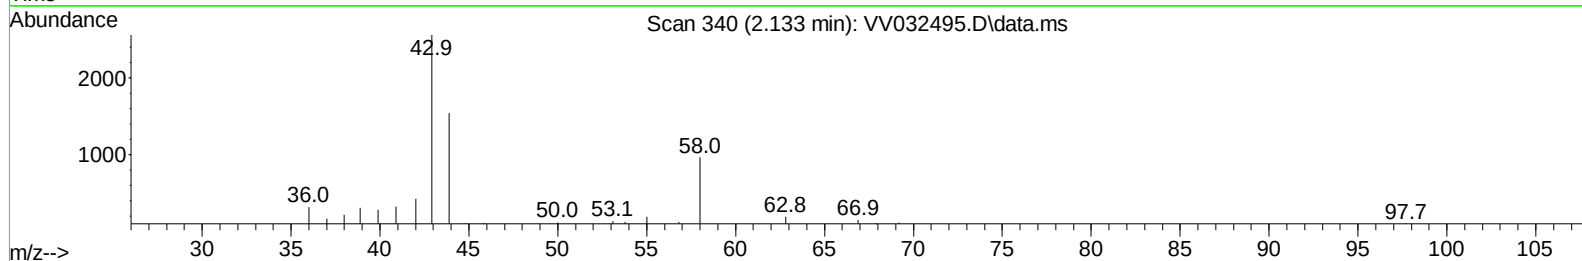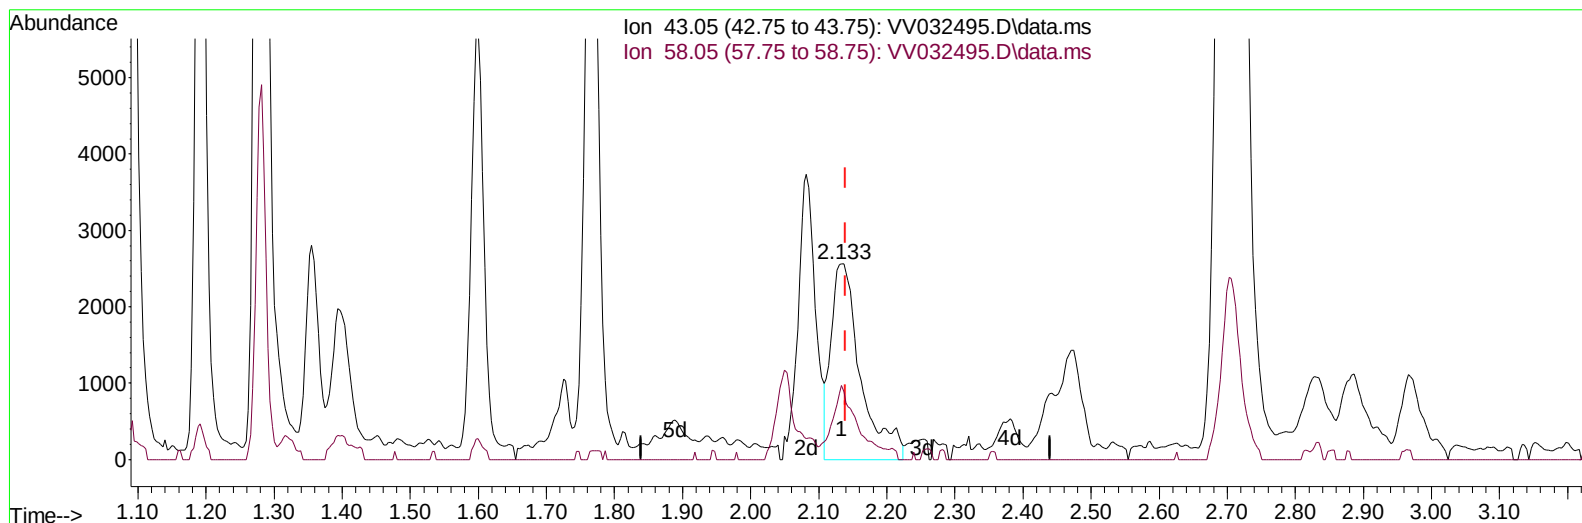

TIC: VV032495.D\data.ms

(13) Acetone (T)

2.133min (-0.006) 4.84 ug/L m

response 7752

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 33.00  | 24.79  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV101923\  
 Data File : VV032495.D  
 Acq On : 19 Oct 2023 14:29  
 Operator : SY/MD  
 Sample : 04918-15  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AH2

Manual IntegrationsAPPROVED

Quant Time: Oct 20 06:22:34 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Oct 20 06:17:42 2023  
 Response via : Initial Calibration

Reviewed By : John Carlone 10/20/2023  
 Supervised By : Mahesh Dadoda 10/24/2023

| Compound                      | R.T.           | QIon | Response   | Conc    | Units | Dev(Min) |
|-------------------------------|----------------|------|------------|---------|-------|----------|
| -----                         |                |      |            |         |       |          |
| Internal Standards            |                |      |            |         |       |          |
| 1) 1,4-Difluorobenzene        | 5.538          | 114  | 101066     | 5.000   | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 8.789          | 117  | 106995     | 5.000   | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.188         | 152  | 50655      | 5.000   | ug/L  | 0.00     |
| System Monitoring Compounds   |                |      |            |         |       |          |
| 4) Vinyl Chloride-d3          | 1.278          | 65   | 35481      | 4.317   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 40 - 130 |      | Recovery = | 86.400% |       |          |
| 7) Chloroethane-d5            | 1.532          | 69   | 32095      | 4.810   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 65 - 130 |      | Recovery = | 96.200% |       |          |
| 11) 1,1-Dichloroethene-d2     | 2.060          | 65   | 14183      | 4.091   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 60 - 125 |      | Recovery = | 81.800% |       |          |
| 20) 2-Butanone-d5             | 3.802          | 46   | 91887      | 44.192  | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 40 - 130 |      | Recovery = | 88.380% |       |          |
| 24) Chloroform-d              | 4.256          | 84   | 60383      | 4.164   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 70 - 125 |      | Recovery = | 83.200% |       |          |
| 26) 1,2-Dichloroethane-d4     | 4.947          | 65   | 31136      | 4.533   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 70 - 130 |      | Recovery = | 90.600% |       |          |
| 32) Benzene-d6                | 4.963          | 84   | 121219     | 3.850   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 70 - 125 |      | Recovery = | 77.000% |       |          |
| 36) 1,2-Dichloropropane-d6    | 5.992          | 67   | 40552      | 3.888   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 60 - 140 |      | Recovery = | 77.800% |       |          |
| 41) Toluene-d8                | 7.246          | 98   | 106314     | 3.693   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 70 - 130 |      | Recovery = | 73.800% |       |          |
| 43) trans-1,3-Dichloroprop... | 7.561          | 79   | 13974      | 3.781   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 55 - 130 |      | Recovery = | 75.600% |       |          |
| 46) 2-Hexanone-d5             | 8.030          | 63   | 75866      | 43.623  | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 45 - 130 |      | Recovery = | 87.240% |       |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.156         | 84   | 32823      | 4.499   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 65 - 120 |      | Recovery = | 90.000% |       |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.564         | 152  | 40942      | 4.356   | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 80 - 120 |      | Recovery = | 87.200% |       |          |
| Target Compounds              |                |      |            |         |       |          |
|                               |                |      |            |         |       | Qvalue   |
| 13) Acetone                   | 2.133          | 43   | 7752m      | 4.837   | ug/L  |          |
| 14) Carbon disulfide          | 2.243          | 76   | 3182       | 0.123   | ug/L  | 99       |
| 17) Methyl tert-butyl Ether   | 2.706          | 73   | 293185     | 14.529  | ug/L  | 98       |
| 33) Benzene                   | 5.018          | 78   | 23889      | 0.634   | ug/L  | 100      |
| 47) Tetrachloroethene         | 7.908          | 164  | 1320       | 0.169   | ug/L  | 87       |
| -----                         |                |      |            |         |       |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV101923\  
Data File : VV032495.D  
Acq On : 19 Oct 2023 14:29  
Operator : SY/MD  
Sample : 04918-15  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AH2

Manual IntegrationsAPPROVED

Quant Time: Oct 20 06:22:34 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Oct 20 06:17:42 2023  
Response via : Initial Calibration

Reviewed By :John Carlone 10/20/2023  
Supervised By :Mahesh Dadoda 10/24/2023

