

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101923\
 Data File : VW032504.D
 Acq On : 19 Oct 2023 18:05
 Operator : SY/MD
 Sample : 04950-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49M3

Quant Time: Oct 20 06:25:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 20 06:17:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	82794	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	92746	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	41395	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	30792	4.573	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.400%
7) Chloroethane-d5	1.532	69	28458	5.207	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.200%
11) 1,1-Dichloroethene-d2	2.060	65	11748	4.137	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.800%
20) 2-Butanone-d5	3.796	46	90082	52.885	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.760%
24) Chloroform-d	4.253	84	56015	4.716	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.400%
26) 1,2-Dichloroethane-d4	4.947	65	31112	5.529	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.600%
32) Benzene-d6	4.963	84	109855	4.025	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.600%
36) 1,2-Dichloropropane-d6	5.992	67	40386	4.467	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.400%
41) Toluene-d8	7.246	98	94435	3.784	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.600%
43) trans-1,3-Dichloroprop...	7.561	79	13713	4.280	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.600%
46) 2-Hexanone-d5	8.027	63	73882	49.009	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.020%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	31805	5.029	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.600%
66) 1,2-Dichlorobenzene-d4	11.564	152	35232	4.587	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.800%
Target Compounds					Qvalue	
13) Acetone	2.127	43	3117	2.374	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032504.D
Acq On : 19 Oct 2023 18:05
Operator : SY/MD
Sample : 04950-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49M3

Quant Time: Oct 20 06:25:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 20 06:17:42 2023
Response via : Initial Calibration

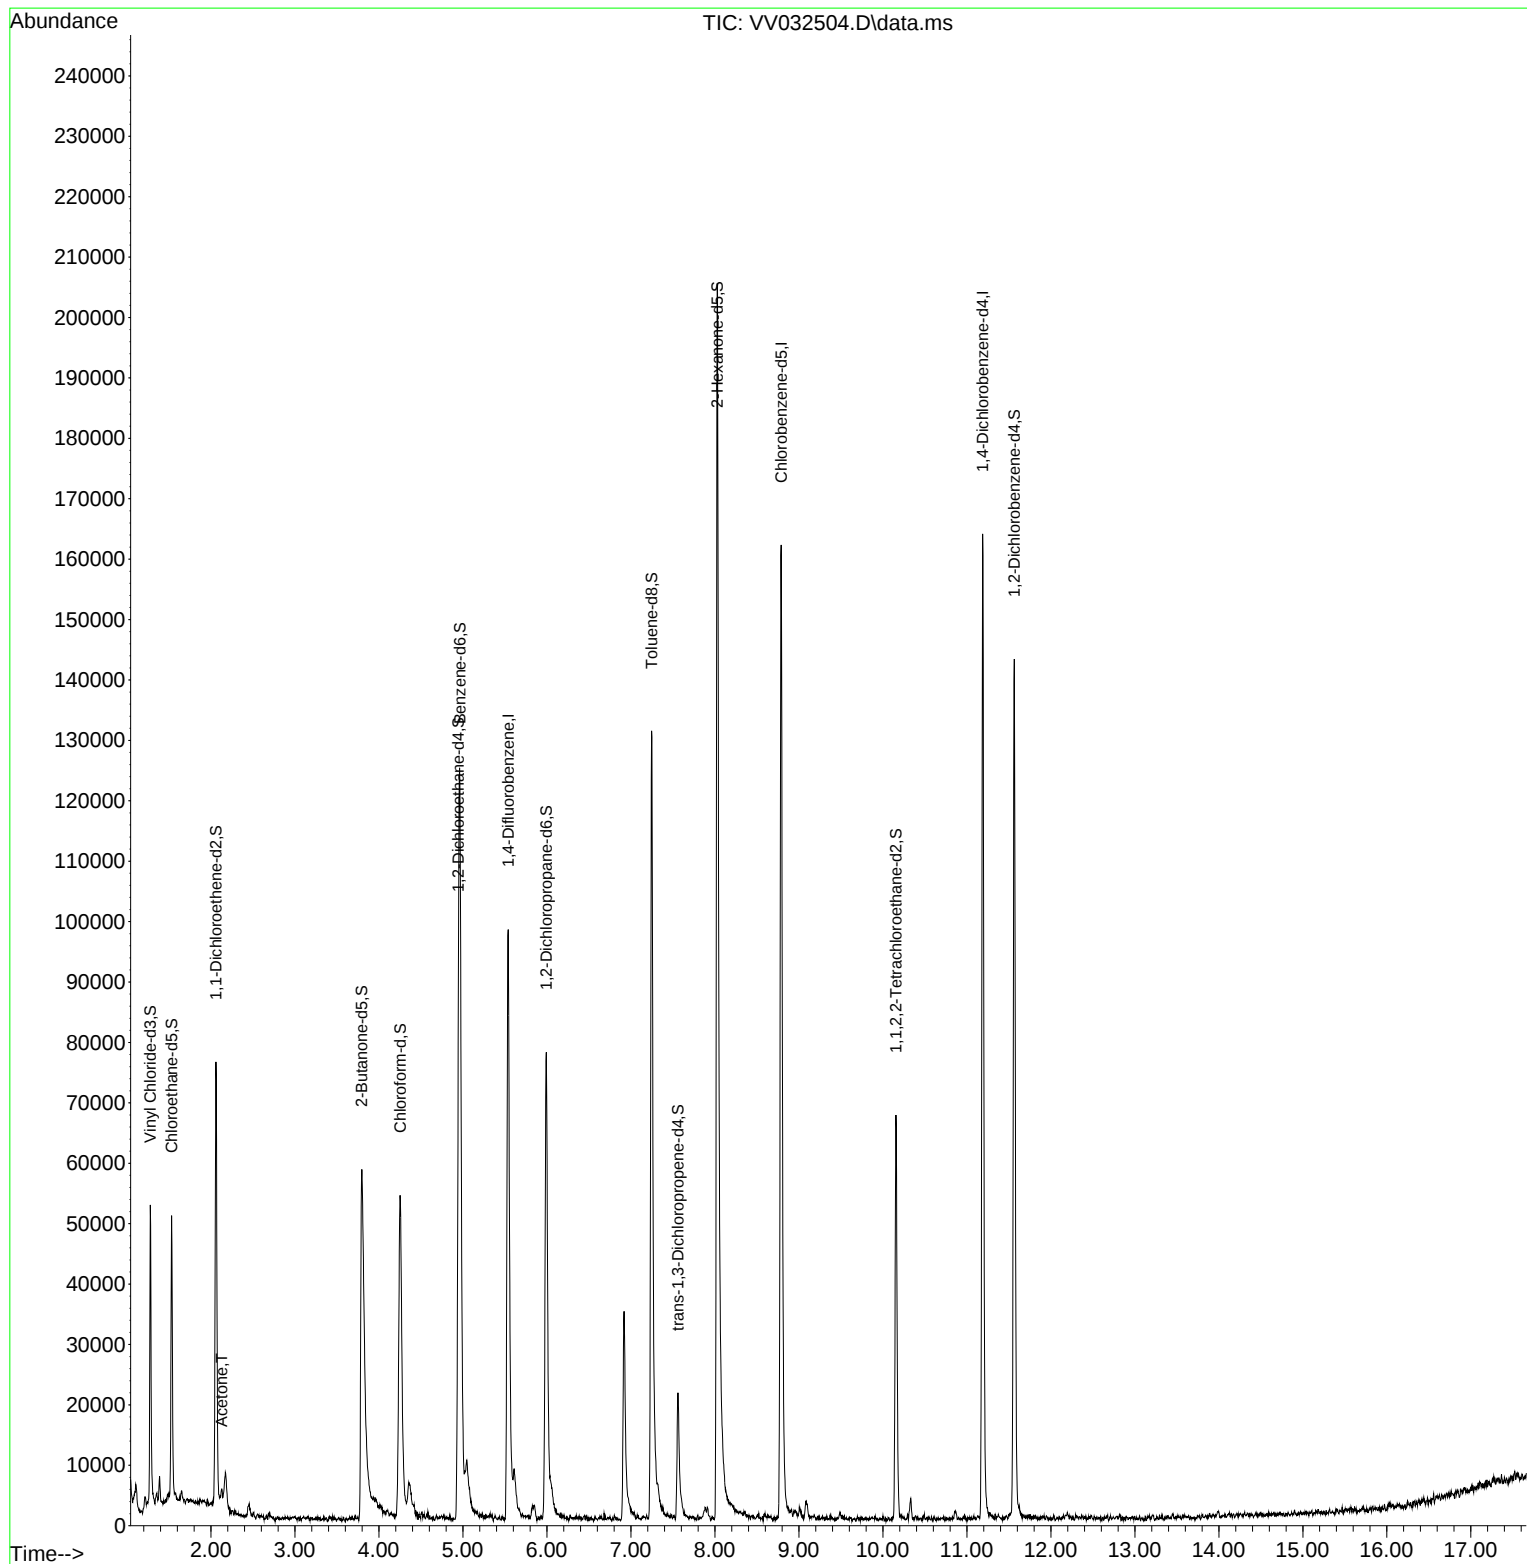

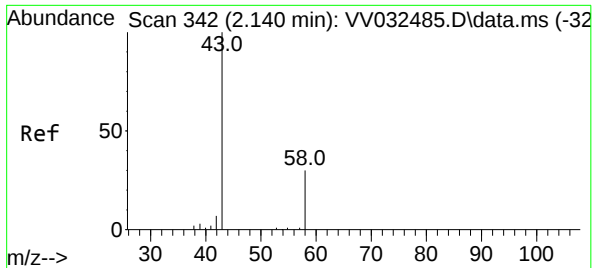

#13
 Acetone
 Concen: 2.374 ug/L
 RT: 2.127 min Scan# 311
 Delta R.T. -0.013 min
 Lab File: VV032504.D
 Acq: 19 Oct 2023 18:05

Instrument :
 MSVOA_V
 ClientSampleId :
 A49M3

Tgt Ion:	43	Resp:	3117
Ion Ratio	Lower	Upper	
43	100		
58	21.6	0.0	66.0

