

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032486.D
 Acq On : 19 Oct 2023 10:11
 Operator : SY/MD
 Sample : VV1019WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK373

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	18	23	31	rVB	5650	8615	1.93%	0.263%
2	1.278	67	74	86	rBV	60413	64311	14.39%	1.966%
3	1.535	145	154	164	rBV	53055	64643	14.47%	1.976%
4	2.060	308	317	339	rVB	89025	136402	30.53%	4.170%
5	2.179	342	354	366	rBV3	7716	15271	3.42%	0.467%
6	2.452	430	439	453	rVB9	2941	5662	1.27%	0.173%
7	3.815	851	863	902	rBV2	39047	159303	35.66%	4.871%
8	4.256	982	1000	1021	rBV	58638	154107	34.49%	4.712%
9	4.368	1025	1035	1052	rVB3	6118	16675	3.73%	0.510%
10	4.960	1202	1219	1240	rBV2	144959	373510	83.60%	11.420%
11	5.539	1387	1399	1415	rBV	105618	225199	50.41%	6.885%
12	5.992	1525	1540	1557	rBV	88431	189720	42.46%	5.801%
13	6.918	1816	1828	1855	rBV	38794	81181	18.17%	2.482%
14	7.246	1918	1930	1961	rBV	156826	311325	69.68%	9.519%
15	7.558	2018	2027	2041	rBV2	22169	43937	9.83%	1.343%
16	8.030	2163	2174	2218	rBV	206007	446777	100.00%	13.660%
17	8.789	2398	2410	2435	rBV	174651	313556	70.18%	9.587%
18	10.156	2825	2835	2850	rBV	68920	112841	25.26%	3.450%
19	11.188	3145	3156	3175	rBV	175394	279849	62.64%	8.556%
20	11.564	3260	3273	3294	rBV	163904	262965	58.86%	8.040%
21	13.448	3852	3859	3866	rBV3	3479	4809	1.08%	0.147%




Sum of corrected areas: 3270658

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032486.D
Acq On : 19 Oct 2023 10:11
Operator : SY/MD
Sample : VV1019WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK373

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

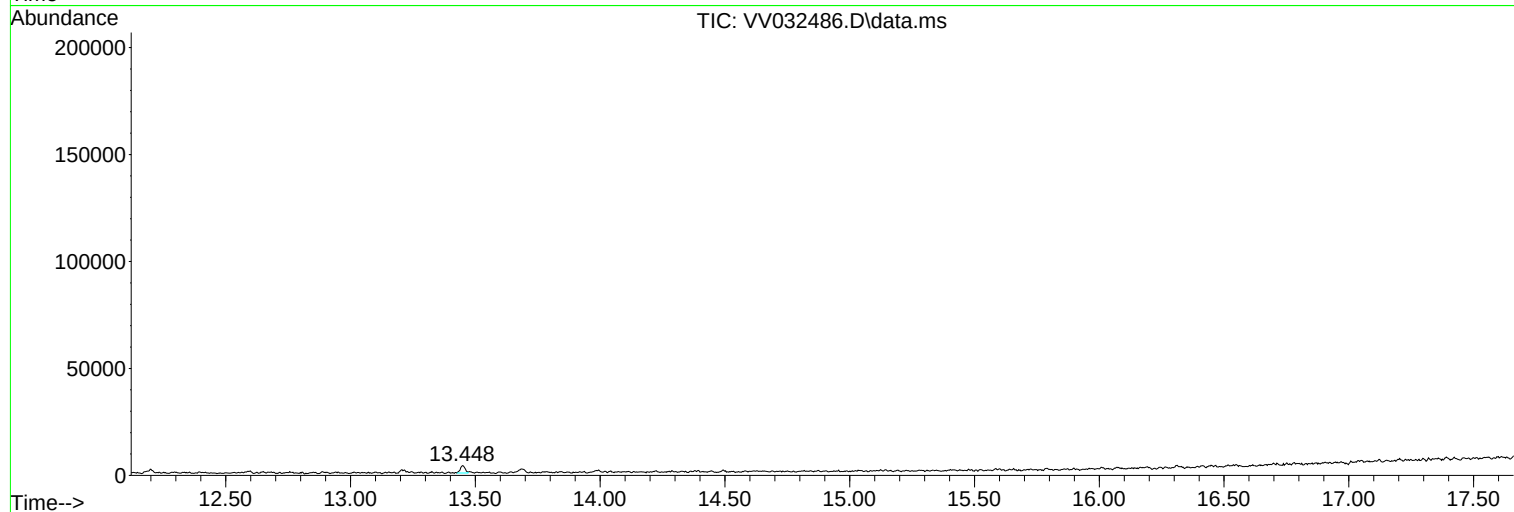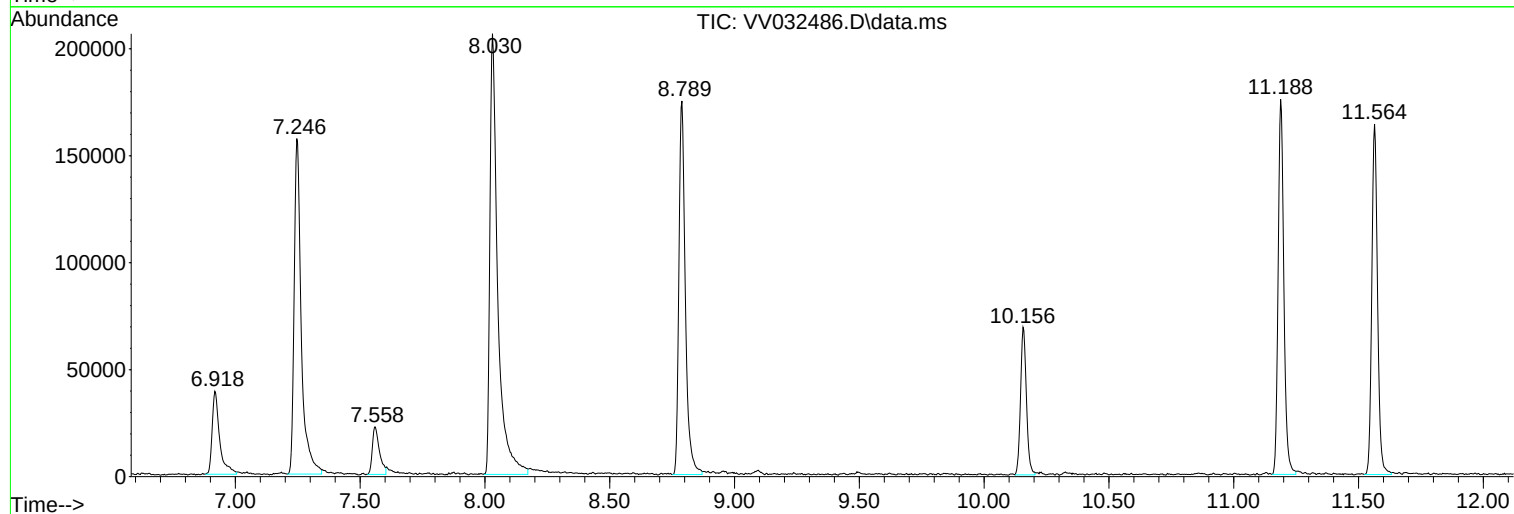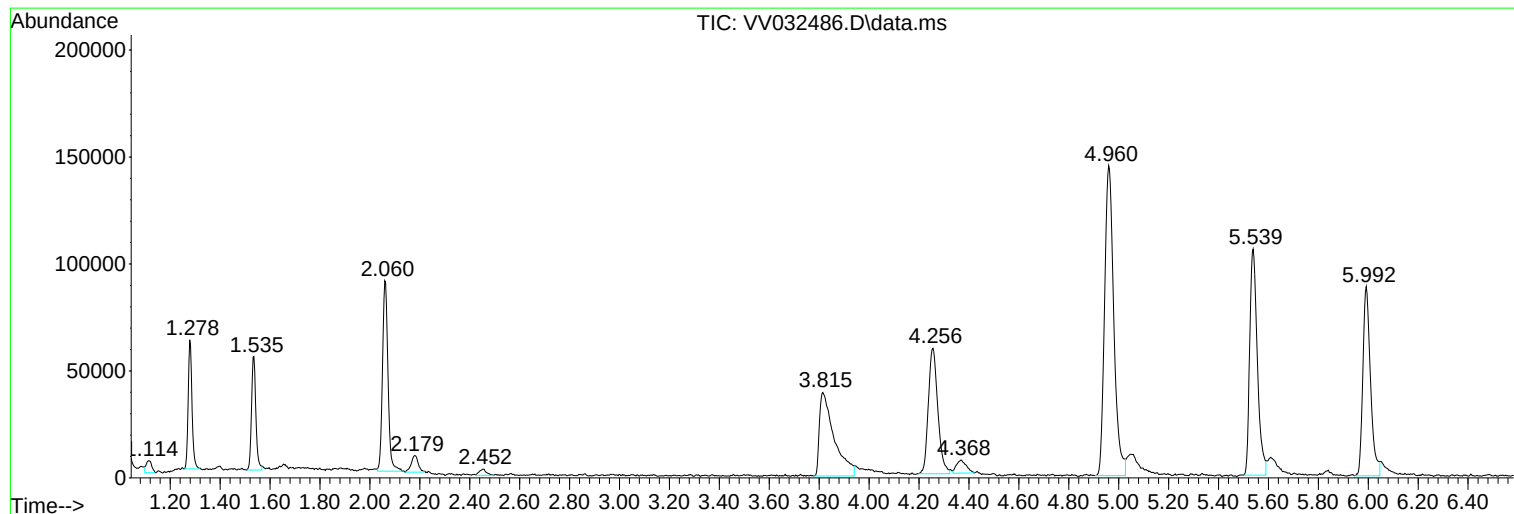

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032486.D
Acq On : 19 Oct 2023 10:11
Operator : SY/MD
Sample : VV1019WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK373

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032486.D
Acq On : 19 Oct 2023 10:11
Operator : SY/MD
Sample : VV1019WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK373

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------