

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032489.D
 Acq On : 19 Oct 2023 12:02
 Operator : SY/MD
 Sample : 04944-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49R8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	11	21	30	rVB2	5916	12642	3.14%	0.374%
2	1.278	67	74	90	rVB	61551	65233	16.18%	1.932%
3	1.388	101	108	116	rVB2	10956	14002	3.47%	0.415%
4	1.532	146	153	166	rVB	51877	60512	15.01%	1.792%
5	2.060	307	317	330	rBV	83966	123144	30.55%	3.647%
6	2.127	333	338	344	rVV4	3826	6016	1.49%	0.178%
7	2.175	346	353	366	rVB3	9401	16815	4.17%	0.498%
8	2.449	428	438	451	rBV2	10285	18392	4.56%	0.545%
9	3.802	844	859	887	rBV3	84266	281884	69.94%	8.349%
10	4.253	981	999	1020	rBV2	55847	150967	37.46%	4.471%
11	4.362	1025	1033	1034	rBV2	4055	4540	1.13%	0.134%
12	4.960	1201	1219	1238	rBV2	138713	356590	88.47%	10.562%
13	5.535	1387	1398	1415	rBV	108276	230835	57.27%	6.837%
14	5.992	1527	1540	1557	rBV2	82441	179828	44.62%	5.326%
15	6.918	1818	1828	1848	rBV	37138	75374	18.70%	2.232%
16	7.246	1917	1930	1952	rBV	150845	295294	73.26%	8.746%
17	7.561	2018	2028	2046	rBV	21720	46128	11.44%	1.366%
18	7.876	2117	2126	2132	rBV3	4463	7573	1.88%	0.224%
19	8.027	2162	2173	2211	rBV	189275	403055	100.00%	11.938%
20	8.789	2396	2410	2433	rBV	175700	320749	79.58%	9.500%
21	9.082	2493	2501	2509	rBV10	3984	7172	1.78%	0.212%
22	10.156	2824	2835	2852	rBV	64519	106084	26.32%	3.142%
23	10.329	2879	2889	2900	rVB2	14130	22899	5.68%	0.678%
24	11.188	3145	3156	3172	rBV	184871	293763	72.88%	8.701%
25	11.564	3261	3273	3292	rBV	158124	262891	65.22%	7.786%
26	12.194	3460	3469	3475	rBV3	3580	5121	1.27%	0.152%
27	13.204	3775	3783	3791	rBV6	6105	8797	2.18%	0.261%




Sum of corrected areas: 3376300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032489.D
Acq On : 19 Oct 2023 12:02
Operator : SY/MD
Sample : 04944-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49R8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

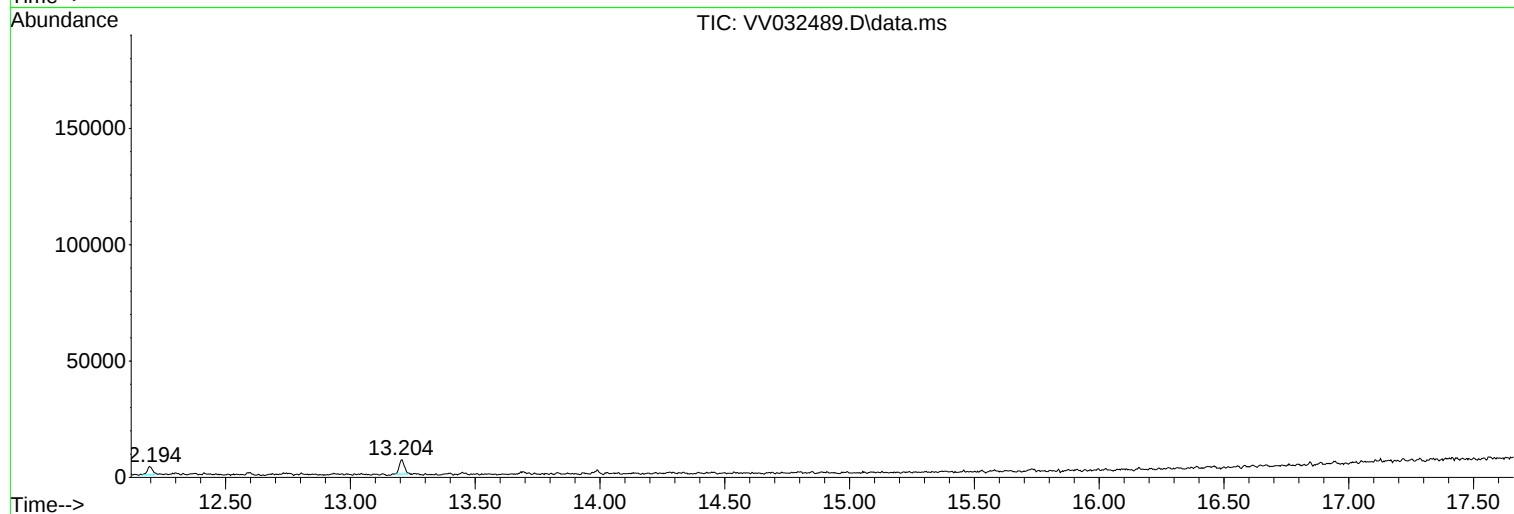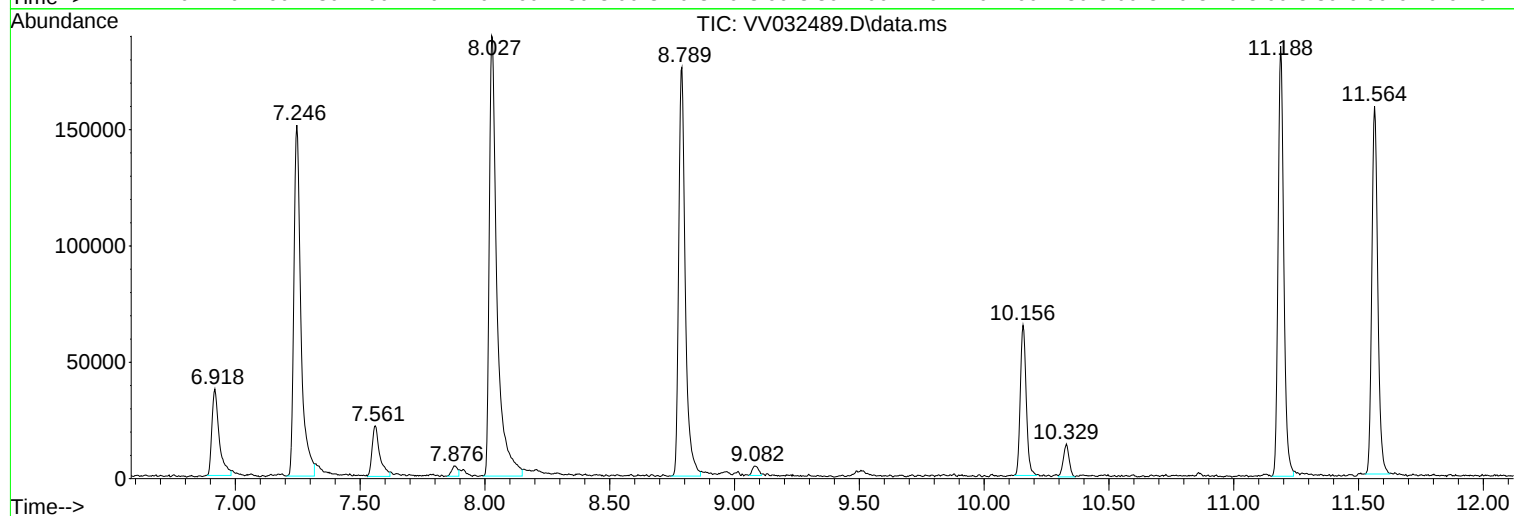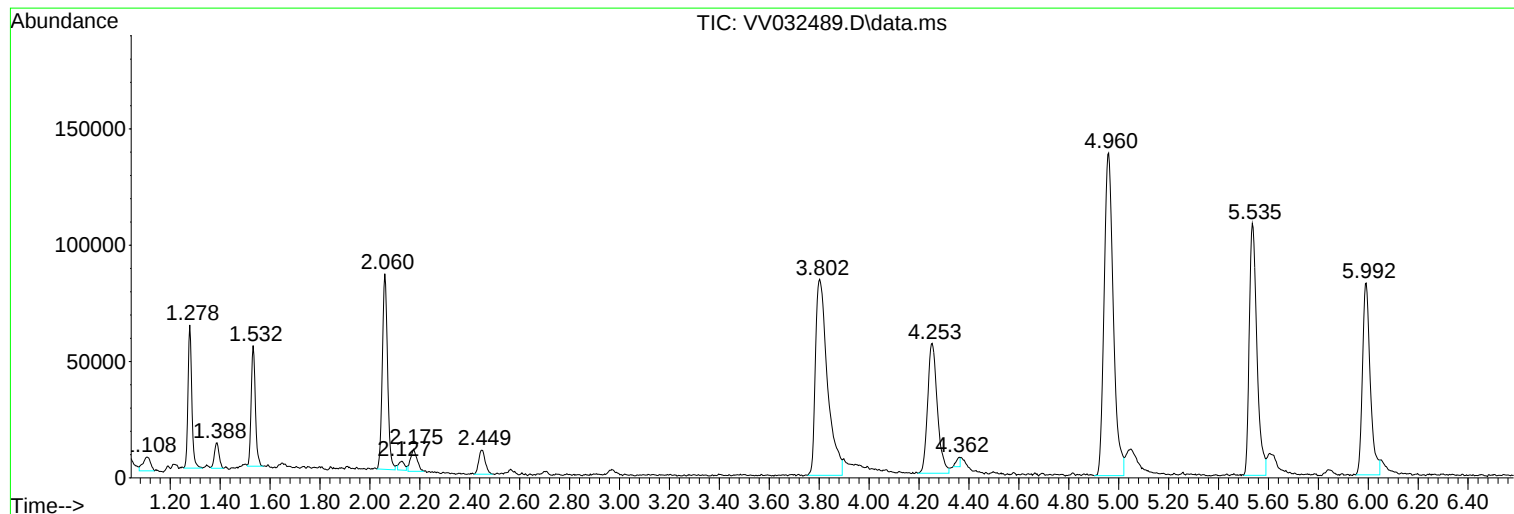

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032489.D
Acq On : 19 Oct 2023 12:02
Operator : SY/MD
Sample : 04944-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49R8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032489.D
Acq On : 19 Oct 2023 12:02
Operator : SY/MD
Sample : 04944-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49R8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc