

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032490.D
 Acq On : 19 Oct 2023 12:27
 Operator : SY/MD
 Sample : 04944-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49S0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	18	23	31	rVB	5389	7231	1.72%	0.207%
2	1.217	48	55	66	rBV	25992	30788	7.32%	0.883%
3	1.278	66	74	87	rVV	59769	64760	15.41%	1.858%
4	1.388	102	108	118	rVB5	6146	8291	1.97%	0.238%
5	1.532	146	153	167	rVB	52997	63453	15.10%	1.821%
6	2.060	307	317	330	rBV	83182	123097	29.29%	3.532%
7	2.182	345	355	368	rVB3	10541	21703	5.16%	0.623%
8	3.799	845	858	889	rBV2	57925	192072	45.70%	5.511%
9	4.252	984	999	1022	rBV2	57004	151457	36.03%	4.346%
10	4.368	1024	1035	1052	rVB3	6672	21202	5.04%	0.608%
11	4.960	1201	1219	1237	rBV2	141480	360529	85.77%	10.345%
12	5.539	1384	1399	1415	rBV	111545	234543	55.80%	6.730%
13	5.992	1524	1540	1556	rBV	86144	185852	44.22%	5.333%
14	6.918	1814	1828	1847	rBV2	36505	78060	18.57%	2.240%
15	7.246	1919	1930	1947	rBV	152178	293345	69.79%	8.417%
16	7.323	1949	1954	1974	rVB	20937	41081	9.77%	1.179%
17	7.561	2015	2028	2046	rBV2	22237	46525	11.07%	1.335%
18	7.883	2118	2128	2134	rBV2	7820	12985	3.09%	0.373%
19	8.027	2163	2173	2206	rBV	200143	420331	100.00%	12.061%
20	8.789	2399	2410	2434	rBV	180207	327835	77.99%	9.407%
21	8.953	2453	2461	2472	rBV	6252	10652	2.53%	0.306%
22	9.079	2491	2500	2514	rBV2	16962	31348	7.46%	0.900%
23	9.487	2616	2627	2639	rBV2	7428	14721	3.50%	0.422%
24	10.156	2823	2835	2852	rBV	67272	113901	27.10%	3.268%
25	10.329	2871	2889	2899	rBV	16415	29650	7.05%	0.851%
26	10.387	2901	2907	2916	rBV6	4155	6930	1.65%	0.199%
27	10.857	3045	3053	3065	rBV3	7827	11968	2.85%	0.343%
28	11.188	3145	3156	3176	rBV	189236	301508	71.73%	8.652%
29	11.564	3262	3273	3297	rVB	165444	272837	64.91%	7.829%
30	12.204	3461	3472	3478	rBV3	3885	6340	1.51%	0.182%




Sum of corrected areas: 3484995

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032490.D
Acq On : 19 Oct 2023 12:27
Operator : SY/MD
Sample : 04944-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

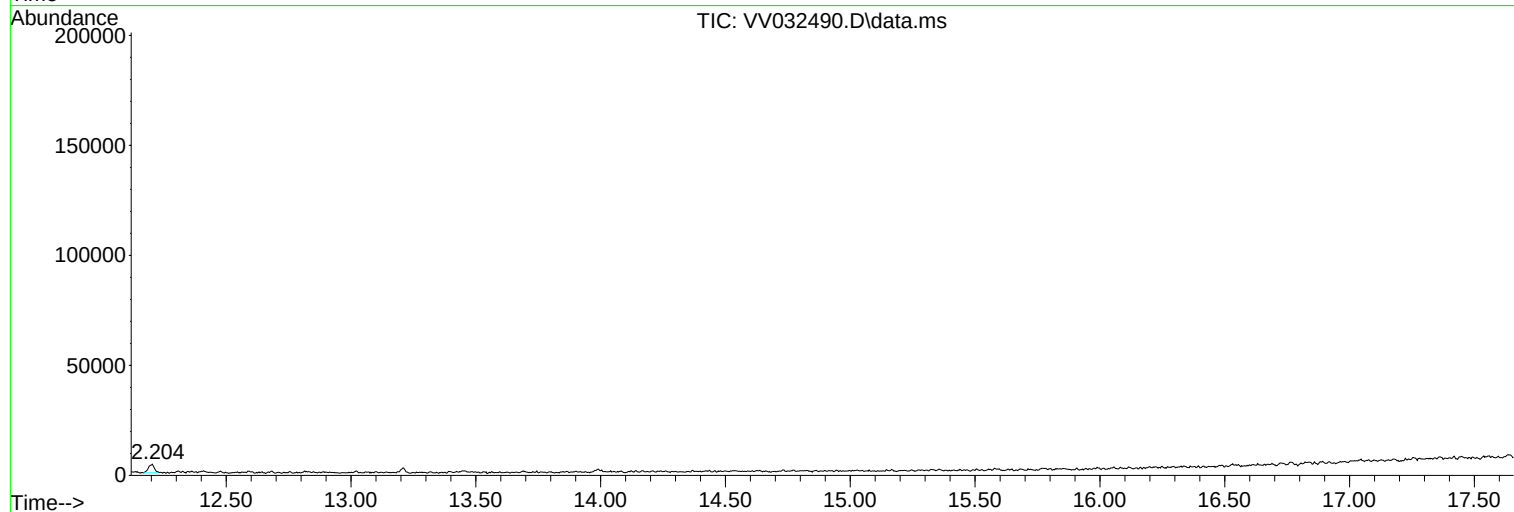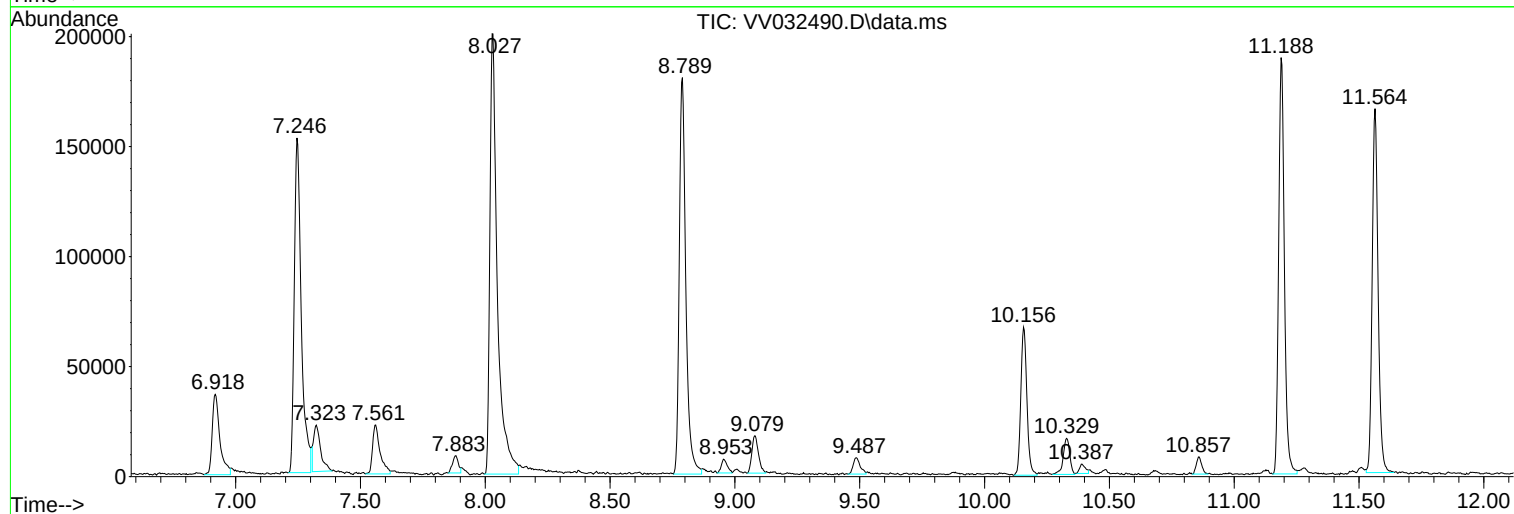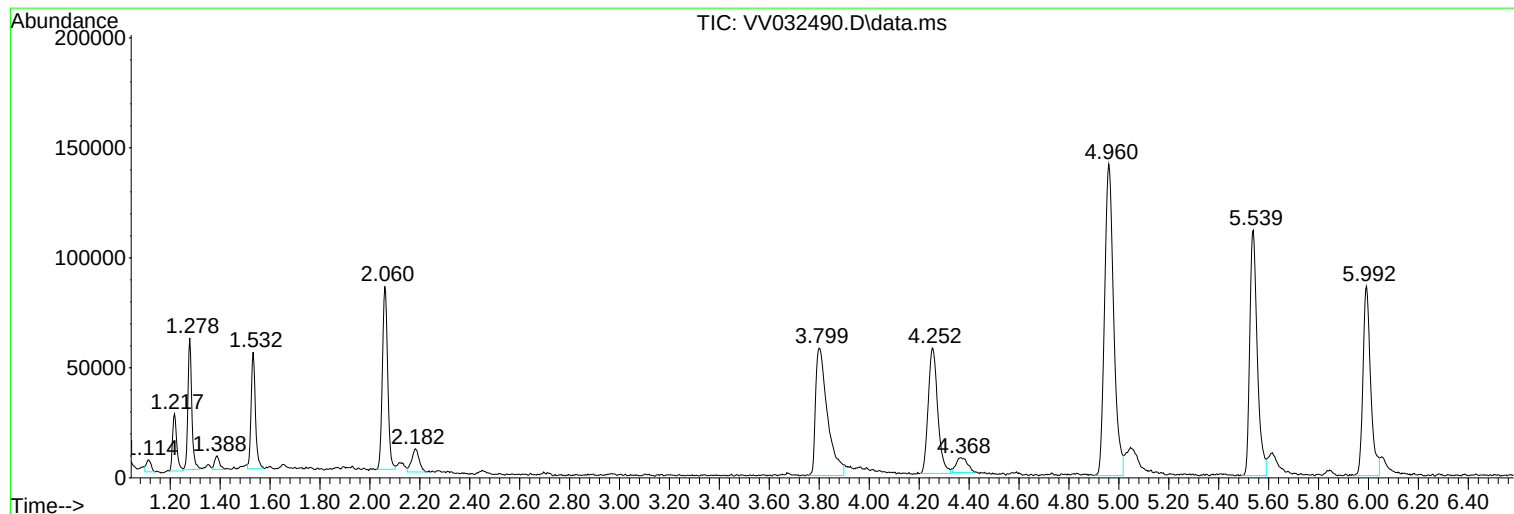

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032490.D
Acq On : 19 Oct 2023 12:27
Operator : SY/MD
Sample : 04944-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032490.D
Acq On : 19 Oct 2023 12:27
Operator : SY/MD
Sample : 04944-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------