

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032491.D
 Acq On : 19 Oct 2023 12:51
 Operator : SY/MD
 Sample : 04944-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49S4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	18	24	31	rVB	5550	8427	2.11%	0.241%
2	1.278	66	74	84	rBV	57767	62054	15.53%	1.776%
3	1.384	101	107	121	rVB	17398	22530	5.64%	0.645%
4	1.532	146	153	168	rVB	52716	61664	15.44%	1.765%
5	2.060	307	317	330	rBV	80819	119916	30.02%	3.431%
6	2.182	346	355	367	rVB2	9256	18893	4.73%	0.541%
7	3.802	841	859	896	rBV2	93147	320490	80.23%	9.171%
8	4.252	984	999	1021	rBV3	54366	148696	37.22%	4.255%
9	4.365	1025	1034	1048	rVV3	7044	17786	4.45%	0.509%
10	4.960	1204	1219	1240	rBV2	139012	364249	91.18%	10.423%
11	5.539	1387	1399	1414	rBV2	107337	225072	56.34%	6.440%
12	5.838	1487	1492	1502	rVB2	2291	4369	1.09%	0.125%
13	5.992	1527	1540	1556	rBV	84101	179327	44.89%	5.131%
14	6.918	1817	1828	1853	rBV	35874	79816	19.98%	2.284%
15	7.246	1919	1930	1947	rBV	148910	290154	72.63%	8.303%
16	7.323	1948	1954	1983	rVB2	23377	53105	13.29%	1.520%
17	7.561	2016	2028	2047	rBV	22851	45871	11.48%	1.313%
18	7.879	2118	2127	2128	rBV6	3443	4140	1.04%	0.118%
19	8.030	2164	2174	2200	rBV	193248	399486	100.00%	11.431%
20	8.789	2399	2410	2433	rBV	178399	318085	79.62%	9.102%
21	8.956	2453	2462	2474	rBV2	6036	9460	2.37%	0.271%
22	9.079	2489	2500	2515	rBV2	16644	31116	7.79%	0.890%
23	9.484	2618	2626	2639	rBV3	7920	14355	3.59%	0.411%
24	10.156	2825	2835	2848	rBV	67768	109937	27.52%	3.146%
25	10.329	2880	2889	2899	rVB5	7906	13189	3.30%	0.377%
26	10.391	2899	2908	2914	rBV6	4429	7150	1.79%	0.205%
27	10.857	3045	3053	3066	rBV2	6989	11366	2.85%	0.325%
28	11.188	3144	3156	3176	rBV	182206	292766	73.29%	8.377%
29	11.564	3262	3273	3296	rVB	161583	261207	65.39%	7.474%




Sum of corrected areas: 3494676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032491.D
Acq On : 19 Oct 2023 12:51
Operator : SY/MD
Sample : 04944-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49S4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

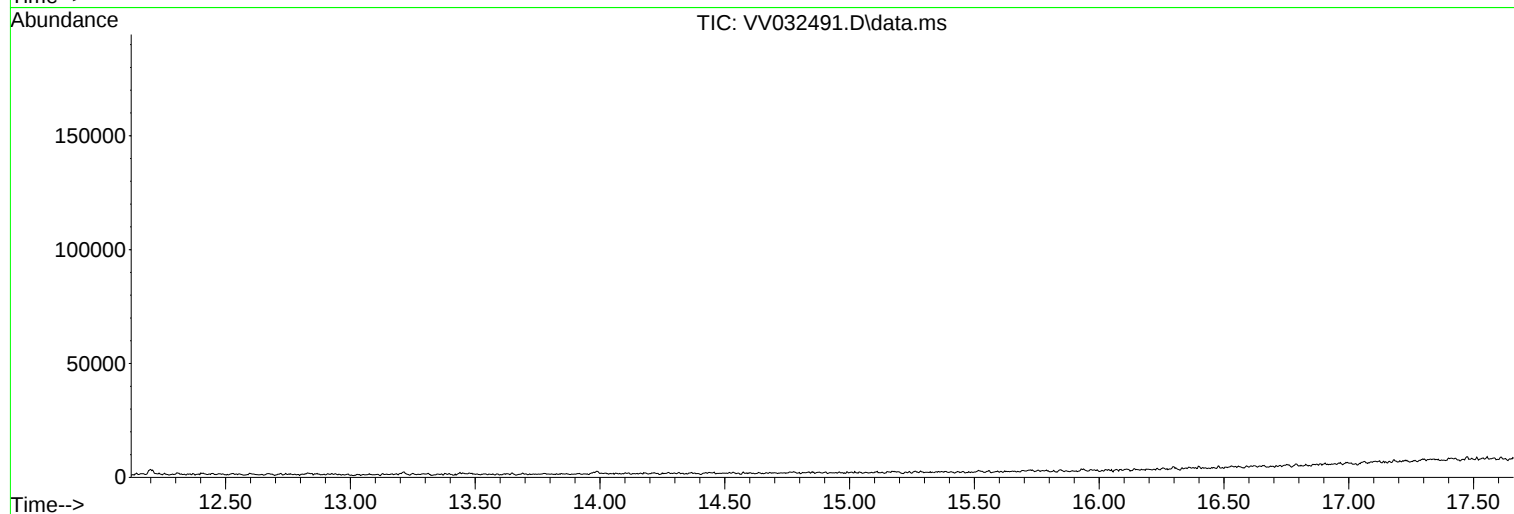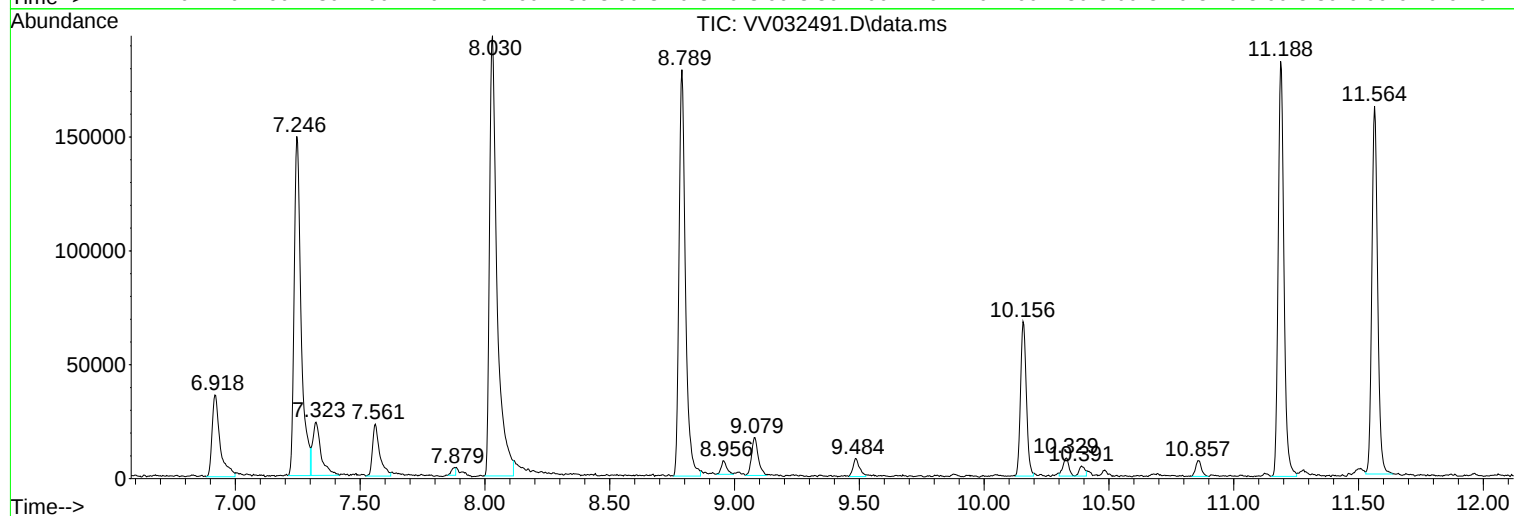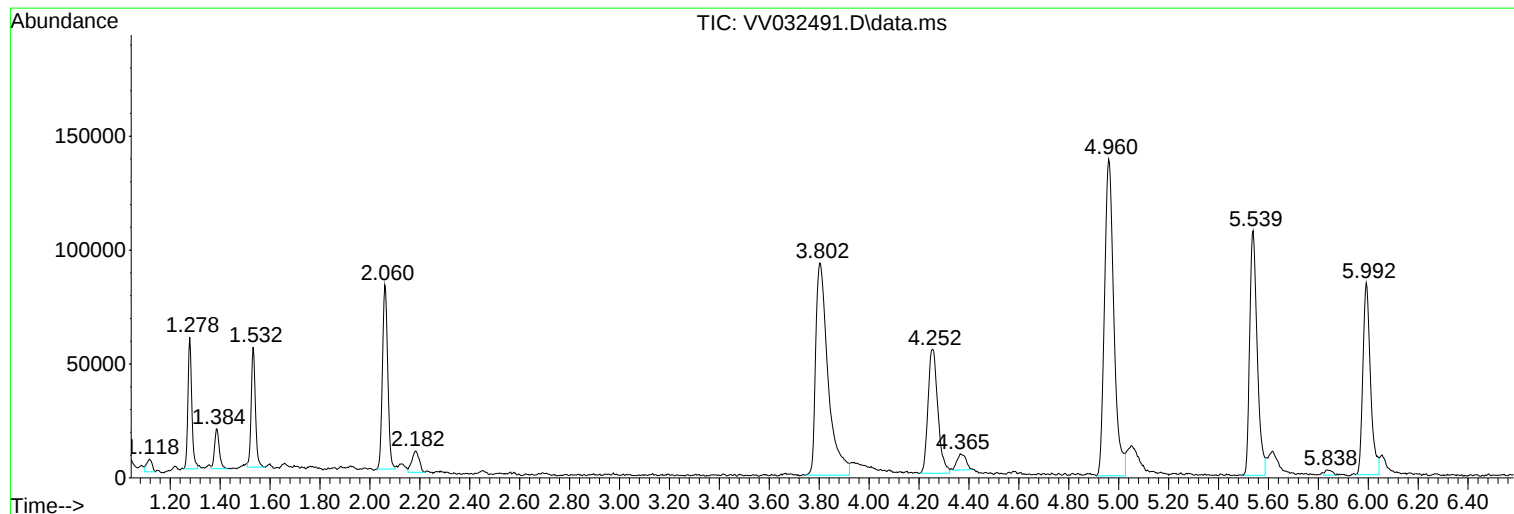

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032491.D
Acq On : 19 Oct 2023 12:51
Operator : SY/MD
Sample : 04944-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49S4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032491.D
Acq On : 19 Oct 2023 12:51
Operator : SY/MD
Sample : 04944-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49S4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc