

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032492.D
 Acq On : 19 Oct 2023 13:16
 Operator : SY/MD
 Sample : 04944-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49S6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	20	24	35	rVB	6224	8115	2.07%	0.248%
2	1.217	49	55	65	rBV	10800	14928	3.82%	0.456%
3	1.278	68	74	88	rVB	54667	59373	15.18%	1.813%
4	1.388	102	108	120	rVB2	9637	12949	3.31%	0.395%
5	1.532	146	153	166	rVV	47484	56409	14.42%	1.722%
6	2.060	307	317	331	rBV	75840	110175	28.17%	3.364%
7	2.182	347	355	369	rVB3	10299	21384	5.47%	0.653%
8	3.805	845	860	885	rBV3	64570	213928	54.69%	6.532%
9	4.256	983	1000	1023	rBV	52776	142671	36.47%	4.356%
10	4.371	1023	1036	1050	rVV4	6869	20155	5.15%	0.615%
11	4.960	1204	1219	1238	rBV2	129219	332779	85.07%	10.160%
12	5.539	1388	1399	1416	rBV	110284	234007	59.82%	7.145%
13	5.992	1528	1540	1555	rBV2	78196	167076	42.71%	5.101%
14	6.921	1819	1829	1850	rBV2	33560	71862	18.37%	2.194%
15	7.249	1919	1931	1948	rBV	139471	274465	70.17%	8.380%
16	7.323	1948	1954	1971	rVB	20452	40912	10.46%	1.249%
17	7.561	2019	2028	2049	rBV2	20726	43643	11.16%	1.333%
18	8.030	2163	2174	2213	rBV	183145	391165	100.00%	11.943%
19	8.789	2398	2410	2439	rBV	181638	331013	84.62%	10.106%
20	8.956	2454	2462	2472	rBV3	5361	8911	2.28%	0.272%
21	9.079	2491	2500	2515	rBV	15280	27895	7.13%	0.852%
22	9.487	2617	2627	2636	rBV4	7014	12659	3.24%	0.387%
23	10.156	2825	2835	2849	rBV	63397	103358	26.42%	3.156%
24	10.333	2880	2890	2900	rVB3	5248	9043	2.31%	0.276%
25	10.390	2900	2908	2912	rBV5	4503	6024	1.54%	0.184%
26	10.860	3042	3054	3063	rBV5	7267	12756	3.26%	0.389%
27	11.188	3145	3156	3173	rBV	187106	301586	77.10%	9.208%
28	11.564	3262	3273	3294	rVB2	150364	246025	62.90%	7.512%




Sum of corrected areas: 3275266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032492.D
Acq On : 19 Oct 2023 13:16
Operator : SY/MD
Sample : 04944-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

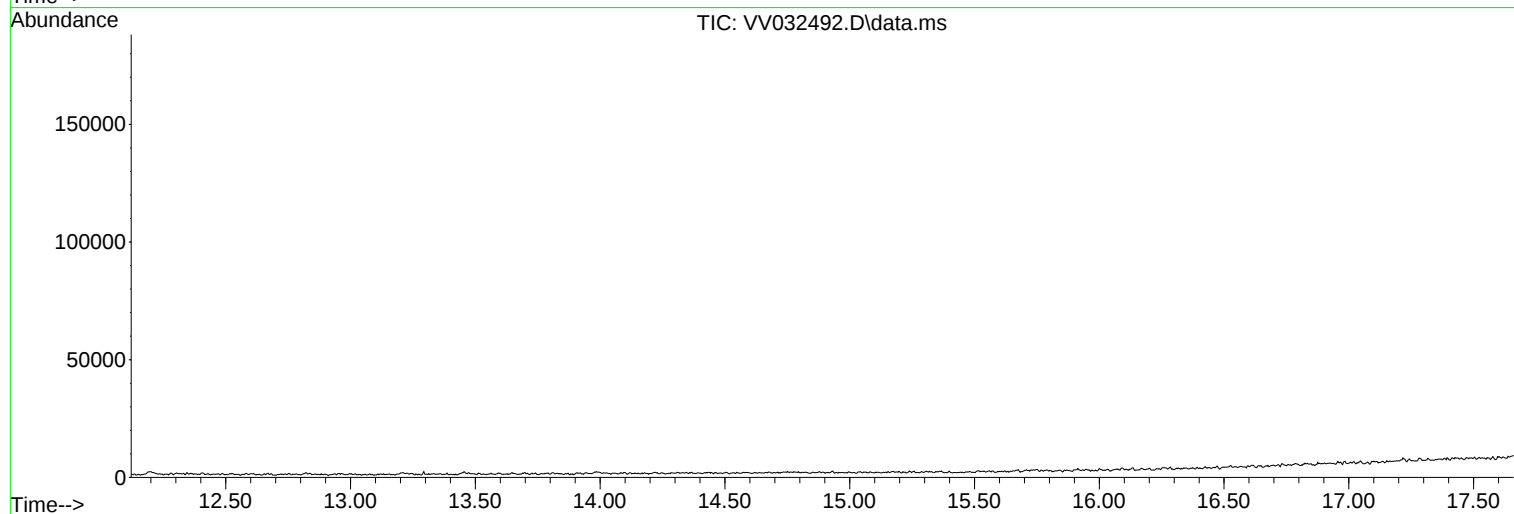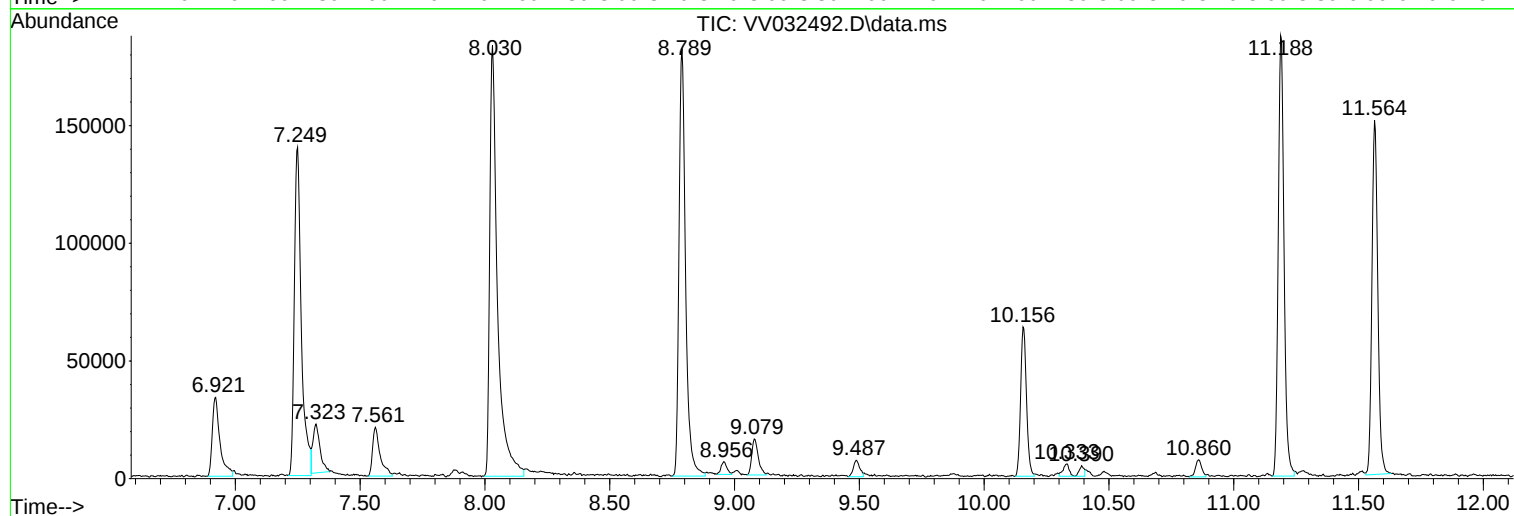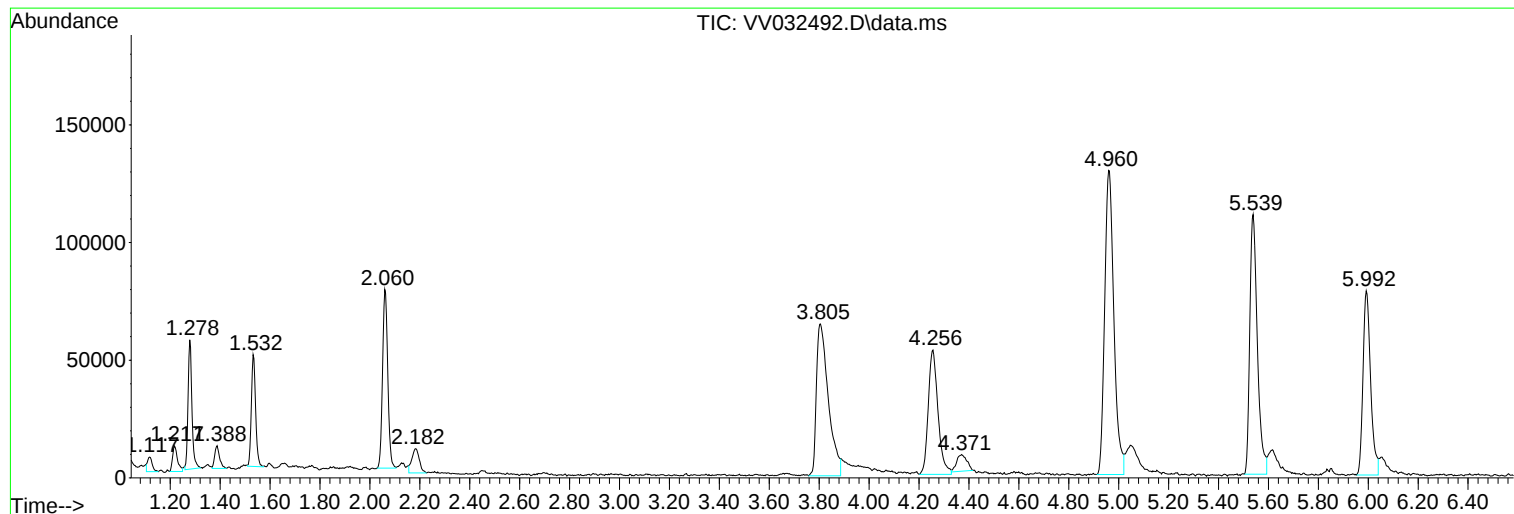

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032492.D
Acq On : 19 Oct 2023 13:16
Operator : SY/MD
Sample : 04944-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032492.D
Acq On : 19 Oct 2023 13:16
Operator : SY/MD
Sample : 04944-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc