

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032497.D
 Acq On : 19 Oct 2023 15:17
 Operator : SY/MD
 Sample : 04944-16DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4AA0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	10	21	31	rVB2	21146	28465	6.15%	0.605%
2	1.282	68	75	87	rBV2	67354	75846	16.40%	1.612%
3	1.536	143	154	156	rBV	53220	58562	12.66%	1.245%
4	2.066	307	319	331	rBV3	137689	244389	52.83%	5.194%
5	2.137	331	341	352	rBV2	33071	81350	17.59%	1.729%
6	2.388	411	419	429	rBV2	6119	11812	2.55%	0.251%
7	2.449	430	438	448	rVB	12271	21134	4.57%	0.449%
8	2.699	505	516	526	rBV	16589	30539	6.60%	0.649%
9	3.117	633	646	659	rBV	9640	22279	4.82%	0.474%
10	3.815	850	863	886	rBV2	55725	182997	39.56%	3.889%
11	4.159	956	970	984	rBV4	13589	36885	7.97%	0.784%
12	4.259	985	1001	1023	rBV3	66726	222136	48.02%	4.721%
13	4.519	1069	1082	1097	rVB4	9914	25229	5.45%	0.536%
14	4.741	1131	1151	1166	rBV2	13212	33307	7.20%	0.708%
15	4.963	1202	1220	1238	rBV3	131744	343311	74.22%	7.297%
16	5.539	1383	1399	1415	rBV	116731	247155	53.43%	5.253%
17	5.841	1482	1493	1512	rBV5	16024	37121	8.02%	0.789%
18	5.992	1524	1540	1575	rBV2	81868	187568	40.55%	3.986%
19	6.918	1817	1828	1836	rBV	37929	68108	14.72%	1.448%
20	6.963	1837	1842	1869	rVB2	23603	48924	10.58%	1.040%
21	7.162	1894	1904	1920	rBV	109549	219811	47.52%	4.672%
22	7.246	1920	1930	1960	rVB	160907	315849	68.28%	6.713%
23	7.558	2018	2027	2035	rBV2	22699	42375	9.16%	0.901%
24	7.776	2086	2095	2112	rBV6	10975	21237	4.59%	0.451%
25	7.908	2117	2136	2156	rVB3	25089	65635	14.19%	1.395%
26	8.030	2162	2174	2204	rBV	202243	418669	90.51%	8.898%
27	8.291	2245	2255	2265	rBV	10752	20087	4.34%	0.427%
28	8.789	2398	2410	2435	rBV2	195918	462571	100.00%	9.831%
29	9.673	2674	2685	2698	rVB3	6249	12187	2.63%	0.259%
30	10.156	2821	2835	2852	rBV	66539	117814	25.47%	2.504%
31	10.329	2877	2889	2900	rBV3	12649	21501	4.65%	0.457%
32	10.853	3040	3052	3066	rBV	57695	90859	19.64%	1.931%
33	11.124	3126	3136	3146	rBV2	34595	57449	12.42%	1.221%
34	11.188	3146	3156	3179	rVB	208201	362234	78.31%	7.699%
35	11.564	3260	3273	3288	rBV	158395	255206	55.17%	5.424%
36	12.201	3461	3471	3482	rVB	5214	8691	1.88%	0.185%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032497.D
Acq On : 19 Oct 2023 15:17
Operator : SY/MD
Sample : 04944-16DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4AA0DL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0

37	12.587	3581	3591	3608	rVB	59617	91512	19.78%	1.945%
38	13.201	3773	3782	3795	rBV	47242	73589	15.91%	1.564%
39	13.683	3923	3932	3947	rBV2	25637	40732	8.81%	0.866%




Sum of corrected areas: 4705125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032497.D
Acq On : 19 Oct 2023 15:17
Operator : SY/MD
Sample : 04944-16DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4AA0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

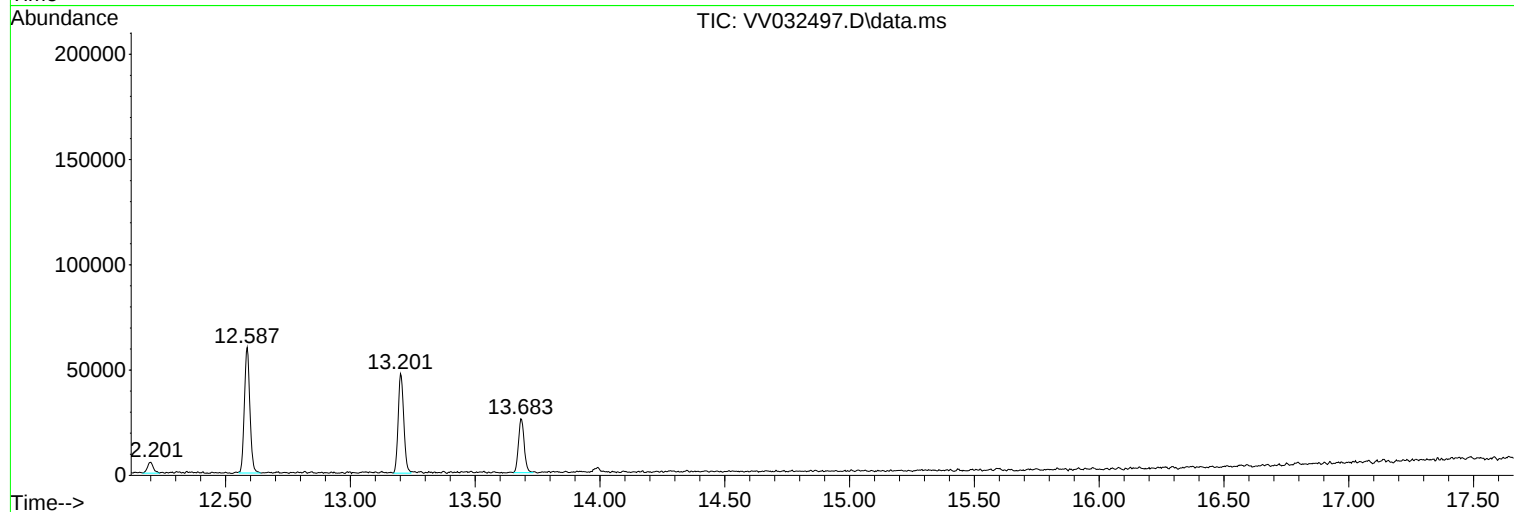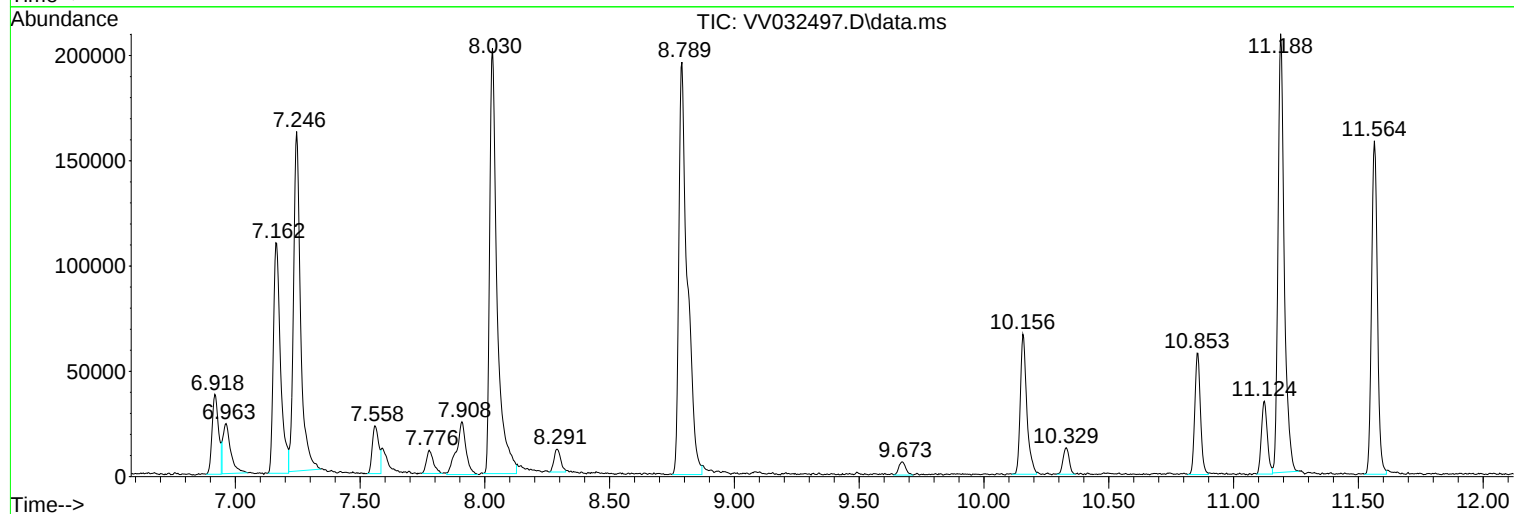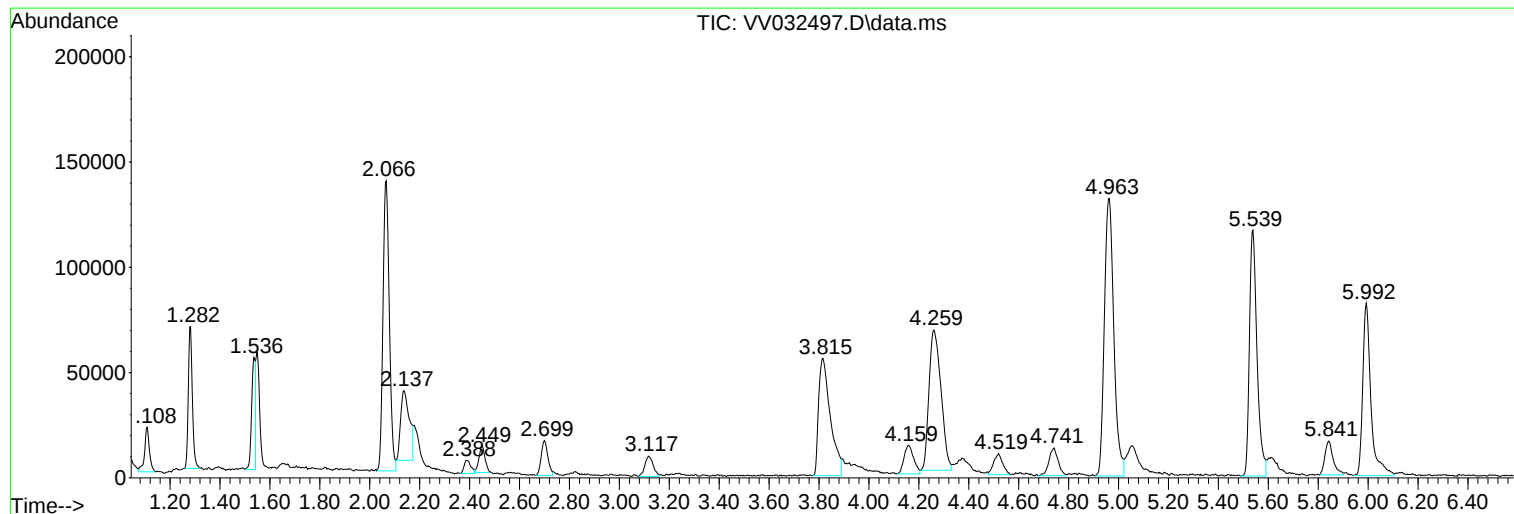

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032497.D
Acq On : 19 Oct 2023 15:17
Operator : SY/MD
Sample : 04944-16DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4AA0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032497.D
Acq On : 19 Oct 2023 15:17
Operator : SY/MD
Sample : 04944-16DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4AA0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc