

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032498.D
 Acq On : 19 Oct 2023 15:42
 Operator : SY/MD
 Sample : 04961-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LJ0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032498.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	87	rBV	57611	62332	14.42%	1.846%
2	1.536	146	154	164	rBV	50726	59322	13.73%	1.757%
3	2.060	307	317	334	rBV	83368	123166	28.50%	3.648%
4	2.179	346	354	367	rVB2	7705	15145	3.50%	0.449%
5	3.815	849	863	903	rBV2	41432	168175	38.92%	4.981%
6	4.256	985	1000	1021	rBV3	58586	161308	37.33%	4.778%
7	4.960	1203	1219	1239	rBV3	142306	370799	85.81%	10.982%
8	5.539	1386	1399	1415	rBV	114678	244840	56.66%	7.252%
9	5.992	1528	1540	1576	rBV2	84755	193839	44.86%	5.741%
10	6.918	1818	1828	1849	rBV	37603	80299	18.58%	2.378%
11	7.246	1919	1930	1949	rBV	152572	293861	68.00%	8.704%
12	7.323	1949	1954	1969	rVB4	8637	18479	4.28%	0.547%
13	7.558	2018	2027	2042	rBV2	23415	46322	10.72%	1.372%
14	7.876	2114	2126	2142	rBV3	7293	14020	3.24%	0.415%
15	8.031	2165	2174	2206	rBV	203292	432134	100.00%	12.799%
16	8.789	2396	2410	2435	rBV	185793	340114	78.71%	10.073%
17	9.082	2492	2501	2517	rBV4	5929	11759	2.72%	0.348%
18	10.156	2821	2835	2854	rBV	68941	112642	26.07%	3.336%
19	10.329	2879	2889	2897	rVB2	13267	20769	4.81%	0.615%
20	11.188	3145	3156	3173	rBV	196685	310760	71.91%	9.204%
21	11.493	3240	3251	3262	rBV5	7250	17500	4.05%	0.518%
22	11.564	3262	3273	3290	rVB	161253	263133	60.89%	7.793%
23	12.194	3460	3469	3481	rVB2	4238	7526	1.74%	0.223%
24	12.291	3493	3499	3509	rBV8	4993	8097	1.87%	0.240%




Sum of corrected areas: 3376341

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032498.D
Acq On : 19 Oct 2023 15:42
Operator : SY/MD
Sample : 04961-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

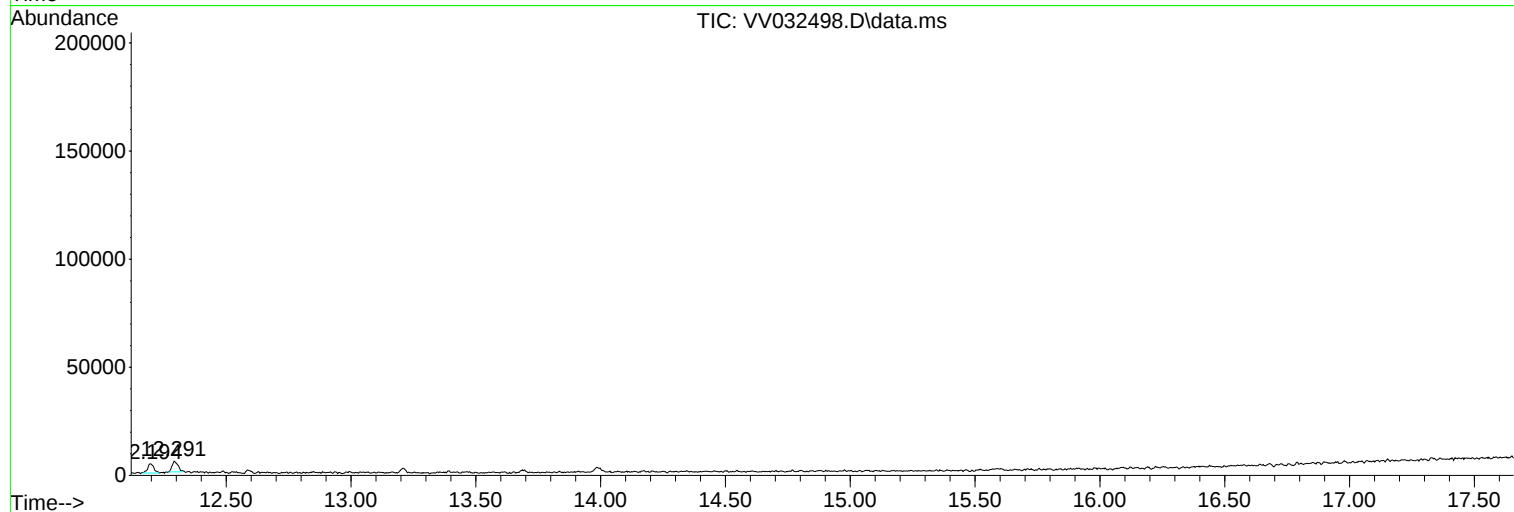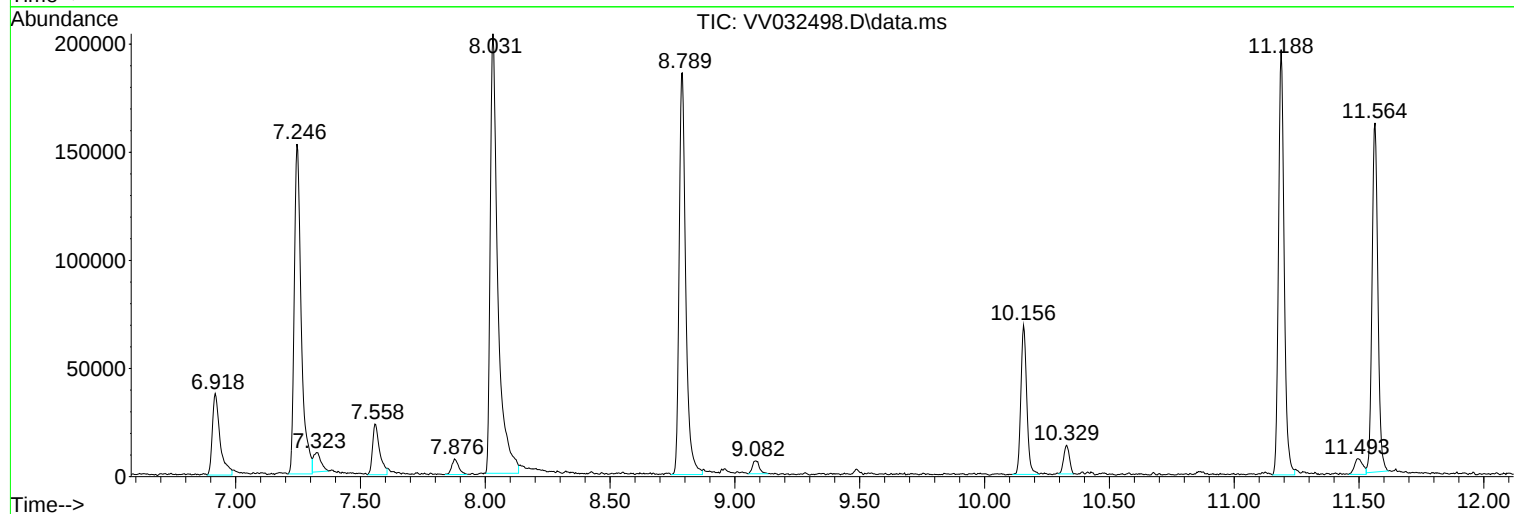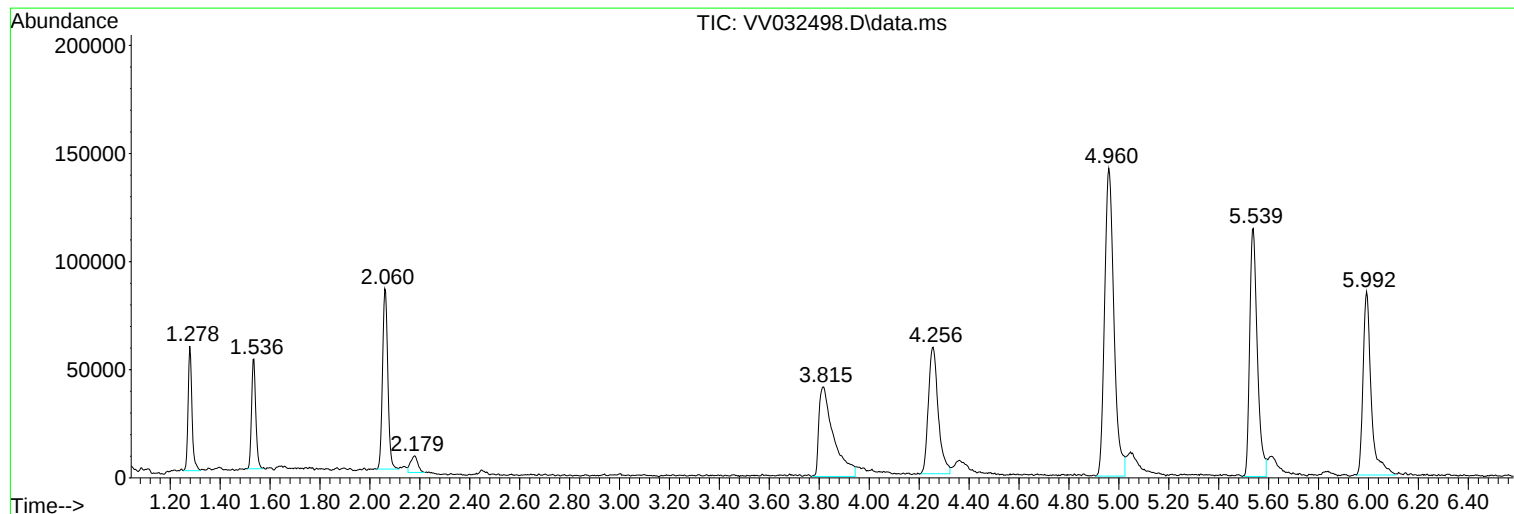

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032498.D
Acq On : 19 Oct 2023 15:42
Operator : SY/MD
Sample : 04961-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032498.D
Acq On : 19 Oct 2023 15:42
Operator : SY/MD
Sample : 04961-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc