

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032501.D
 Acq On : 19 Oct 2023 16:53
 Operator : SY/MD
 Sample : 04950-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49F1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	31	rVB2	4008	6501	1.41%	0.172%
2	1.217	49	55	62	rBV2	4566	5929	1.29%	0.156%
3	1.281	66	75	87	rVV	61185	65533	14.24%	1.729%
4	1.388	102	108	118	rVB	24509	28568	6.21%	0.754%
5	1.535	147	154	166	rVB	54676	63536	13.81%	1.677%
6	2.063	306	318	332	rBV	89345	132639	28.83%	3.500%
7	2.133	335	340	347	rVV8	3804	6888	1.50%	0.182%
8	2.182	349	355	369	rVB3	7271	13850	3.01%	0.366%
9	3.812	842	862	898	rBV4	118316	438232	95.24%	11.565%
10	4.256	982	1000	1023	rBV	63511	168567	36.63%	4.448%
11	4.368	1023	1035	1051	rVB4	5911	17351	3.77%	0.458%
12	4.960	1204	1219	1239	rBV2	150127	389131	84.57%	10.269%
13	5.538	1386	1399	1417	rBV	118343	249891	54.31%	6.595%
14	5.992	1528	1540	1556	rBV2	91288	194206	42.21%	5.125%
15	6.918	1815	1828	1848	rBV	39172	81165	17.64%	2.142%
16	7.246	1919	1930	1949	rBV	161240	310390	67.46%	8.191%
17	7.561	2018	2028	2048	rBV	23624	49686	10.80%	1.311%
18	7.882	2113	2128	2137	rBV2	8678	17327	3.77%	0.457%
19	8.030	2164	2174	2211	rBV	221320	460130	100.00%	12.143%
20	8.789	2396	2410	2430	rBV	192753	340878	74.08%	8.996%
21	9.085	2495	2502	2512	rVB8	3921	6080	1.32%	0.160%
22	10.156	2823	2835	2855	rBV	71866	119034	25.87%	3.141%
23	10.329	2879	2889	2904	rVB2	17973	29309	6.37%	0.773%
24	11.188	3145	3156	3176	rBV	193834	309895	67.35%	8.178%
25	11.564	3261	3273	3289	rBV	170173	277029	60.21%	7.311%
26	12.197	3461	3470	3478	rBV2	5015	7557	1.64%	0.199%




Sum of corrected areas: 3789302

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032501.D
Acq On : 19 Oct 2023 16:53
Operator : SY/MD
Sample : 04950-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

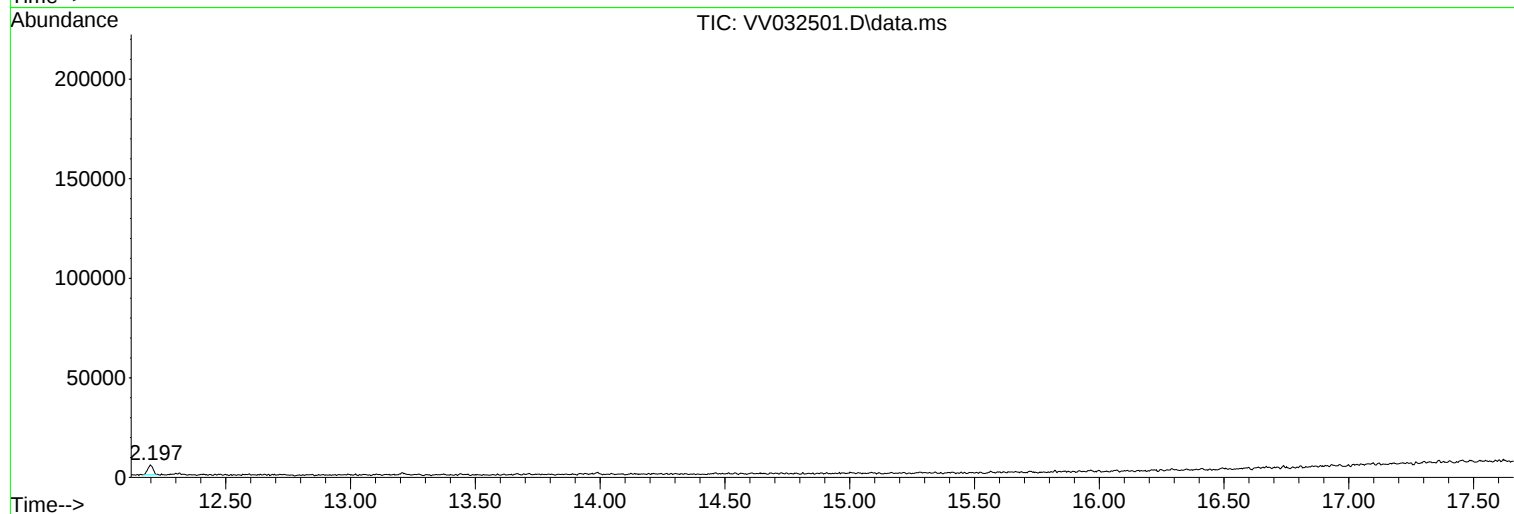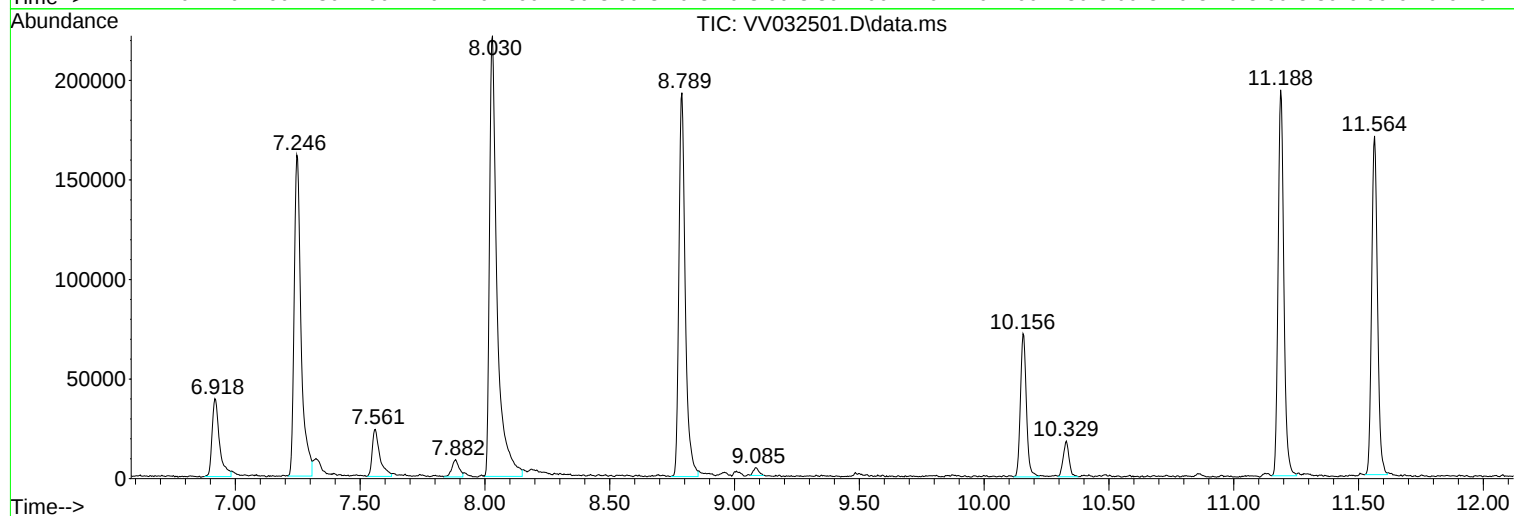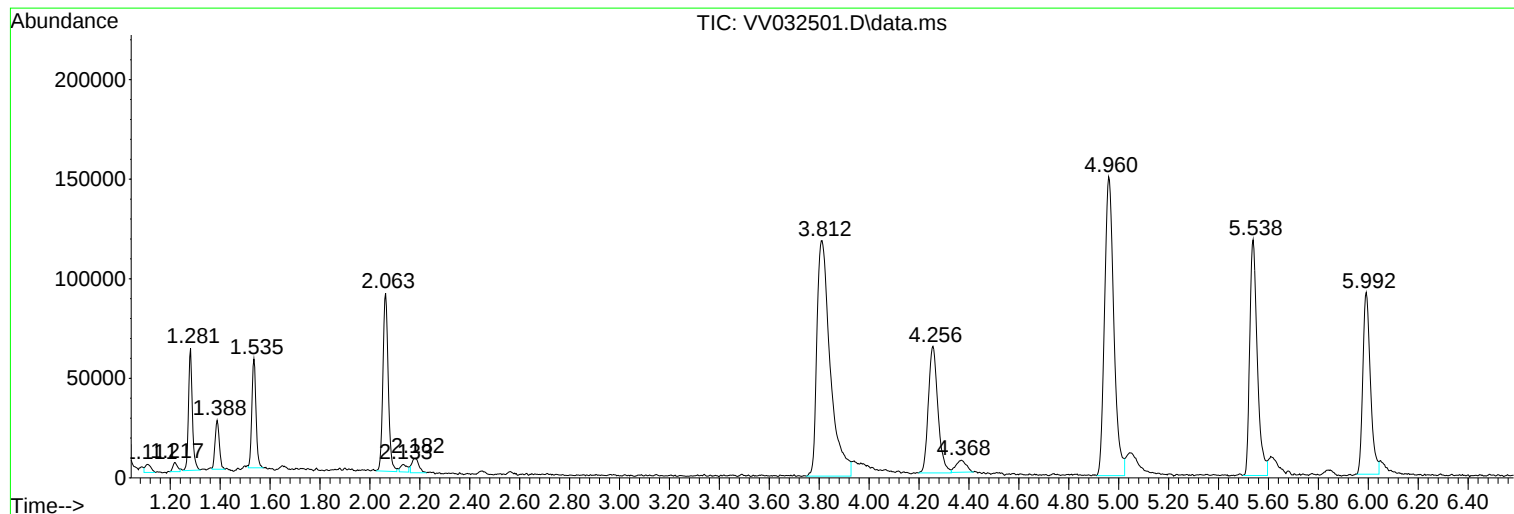

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032501.D
Acq On : 19 Oct 2023 16:53
Operator : SY/MD
Sample : 04950-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032501.D
Acq On : 19 Oct 2023 16:53
Operator : SY/MD
Sample : 04950-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc