

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032504.D
 Acq On : 19 Oct 2023 18:05
 Operator : SY/MD
 Sample : 04950-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49M3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	18	20	32	rVB3	4401	5498	1.29%	0.185%
2	1.217	45	55	59	rBV6	2814	4641	1.09%	0.156%
3	1.278	67	74	91	rVB	49533	54712	12.86%	1.838%
4	1.388	103	108	116	rVB4	4296	4315	1.01%	0.145%
5	1.532	145	153	163	rBV	46409	53511	12.58%	1.798%
6	2.060	307	317	330	rBV	73001	104401	24.54%	3.507%
7	2.172	347	352	363	rVB3	5961	10134	2.38%	0.340%
8	3.796	846	857	893	rBV2	58143	190445	44.76%	6.398%
9	4.253	984	999	1022	rBV3	53000	141411	33.24%	4.750%
10	4.960	1202	1219	1237	rBV2	124429	323311	75.99%	10.861%
11	5.539	1388	1399	1417	rBV	97588	208000	48.89%	6.987%
12	5.992	1526	1540	1568	rBV2	77226	176436	41.47%	5.927%
13	6.918	1815	1828	1853	rBV2	34681	74282	17.46%	2.495%
14	7.246	1918	1930	1950	rBV	130474	254996	59.93%	8.566%
15	7.561	2018	2028	2050	rBV	21023	44892	10.55%	1.508%
16	8.027	2162	2173	2203	rBV	204641	425465	100.00%	14.293%
17	8.789	2398	2410	2432	rBV	161071	289064	67.94%	9.711%
18	9.082	2493	2501	2512	rBV9	3214	6777	1.59%	0.228%
19	10.156	2822	2835	2850	rBV	66911	108187	25.43%	3.634%
20	10.333	2881	2890	2896	rBV5	3585	5424	1.27%	0.182%
21	11.188	3145	3156	3178	rBV	162996	260765	61.29%	8.760%
22	11.564	3259	3273	3287	rBV	141651	230138	54.09%	7.731%




Sum of corrected areas: 2976805

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032504.D
Acq On : 19 Oct 2023 18:05
Operator : SY/MD
Sample : 04950-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49M3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

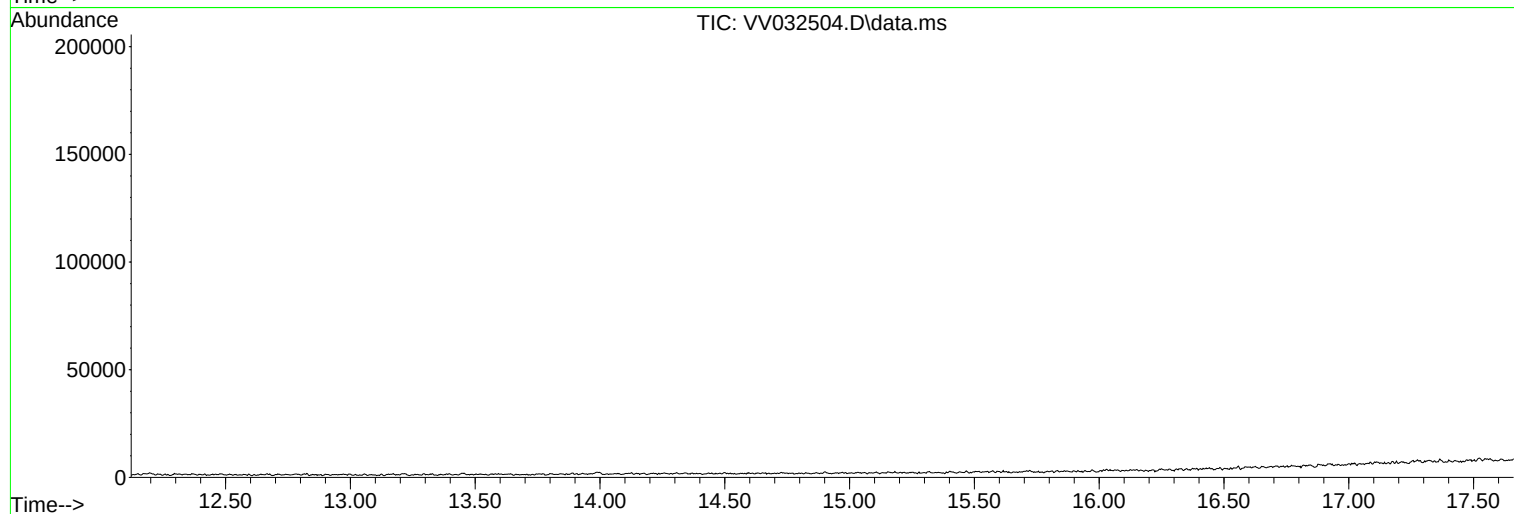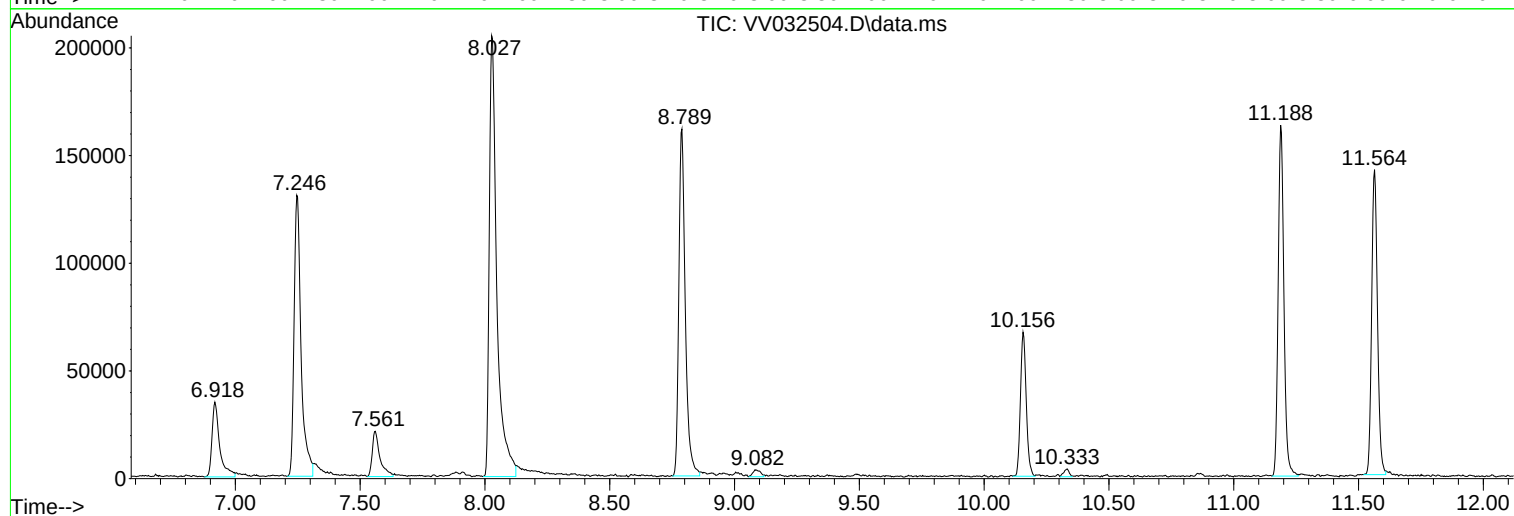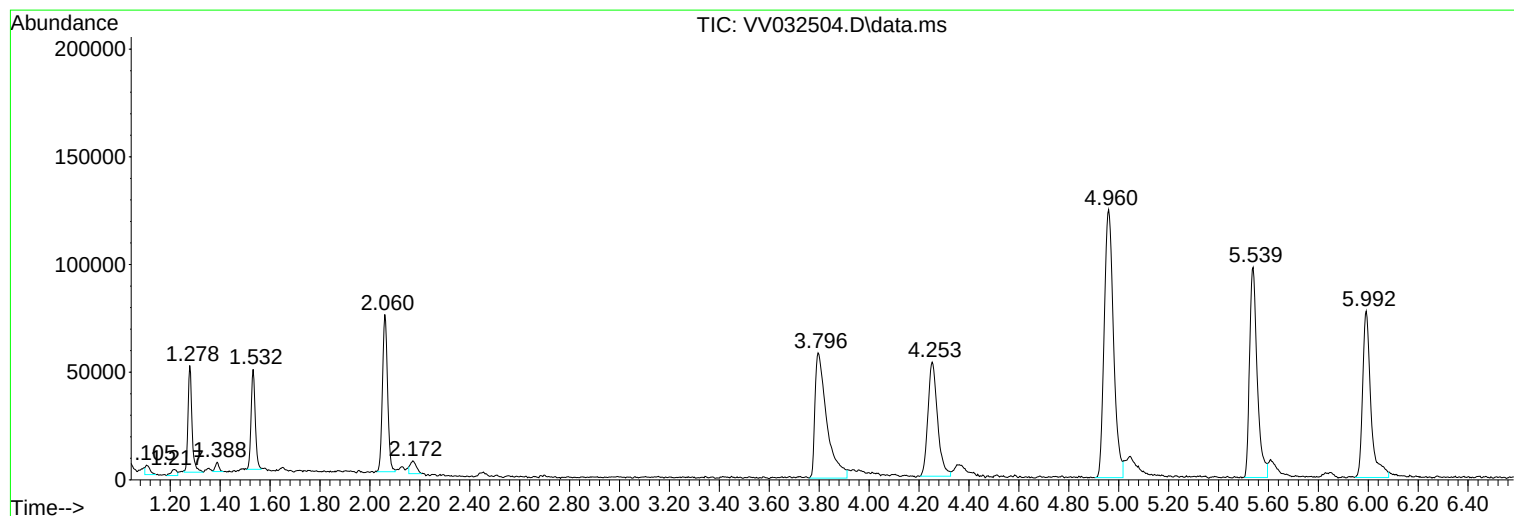

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032504.D
Acq On : 19 Oct 2023 18:05
Operator : SY/MD
Sample : 04950-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49M3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032504.D
Acq On : 19 Oct 2023 18:05
Operator : SY/MD
Sample : 04950-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49M3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc