

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
 Data File : VV032505.D
 Acq On : 19 Oct 2023 18:30
 Operator : SY/MD
 Sample : 04950-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49M0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032505.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	32	rVB2	3768	6052	1.47%	0.191%
2	1.217	49	55	64	rBV	19130	22172	5.37%	0.698%
3	1.278	66	74	85	rBV	53776	58903	14.27%	1.854%
4	1.388	103	108	118	rVB2	7390	9112	2.21%	0.287%
5	1.532	146	153	166	rVB	48862	58255	14.11%	1.834%
6	2.060	308	317	329	rBV	78112	113925	27.59%	3.586%
7	3.806	848	860	893	rBV3	57465	201262	48.75%	6.336%
8	4.253	982	999	1022	rBV2	56930	151294	36.64%	4.763%
9	4.362	1022	1033	1035	rBV5	3476	5449	1.32%	0.172%
10	4.960	1203	1219	1237	rBV3	136945	345375	83.65%	10.872%
11	5.535	1387	1398	1416	rBV	105108	224277	54.32%	7.060%
12	5.992	1525	1540	1556	rBV	81519	175673	42.55%	5.530%
13	6.918	1815	1828	1851	rBV	36088	75362	18.25%	2.372%
14	7.246	1919	1930	1949	rBV	142000	273746	66.30%	8.617%
15	7.558	2015	2027	2038	rBV2	21486	40136	9.72%	1.263%
16	8.031	2164	2174	2207	rBV	193426	412879	100.00%	12.997%
17	8.786	2394	2409	2430	rBV	177181	315123	76.32%	9.920%
18	8.960	2454	2463	2470	rBV7	2663	4264	1.03%	0.134%
19	9.008	2470	2478	2487	rVB5	3560	5746	1.39%	0.181%
20	9.082	2493	2501	2512	rBV5	6945	10996	2.66%	0.346%
21	9.487	2620	2627	2634	rBV6	3151	4476	1.08%	0.141%
22	10.156	2822	2835	2850	rBV	66474	107411	26.02%	3.381%
23	10.329	2882	2889	2898	rVB6	3546	5724	1.39%	0.180%
24	11.188	3144	3156	3177	rBV	177773	288543	69.89%	9.083%
25	11.493	3243	3251	3261	rBV10	5555	12335	2.99%	0.388%
26	11.564	3262	3273	3291	rVB	154532	248213	60.12%	7.814%




Sum of corrected areas: 3176703

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032505.D
Acq On : 19 Oct 2023 18:30
Operator : SY/MD
Sample : 04950-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49M0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

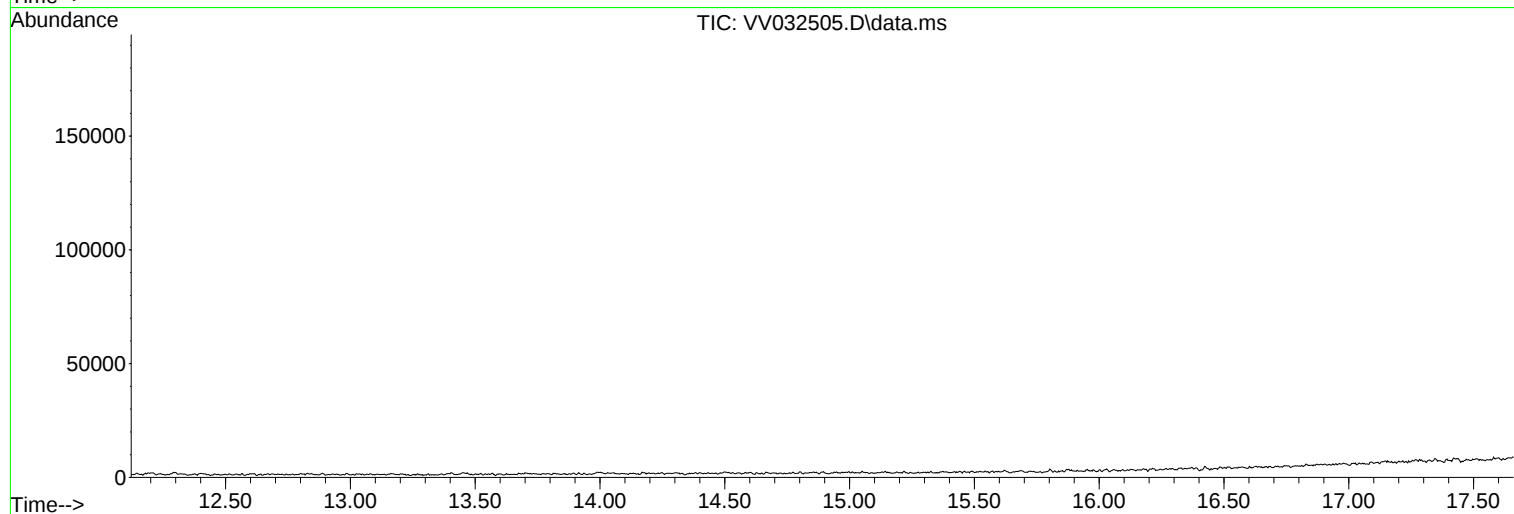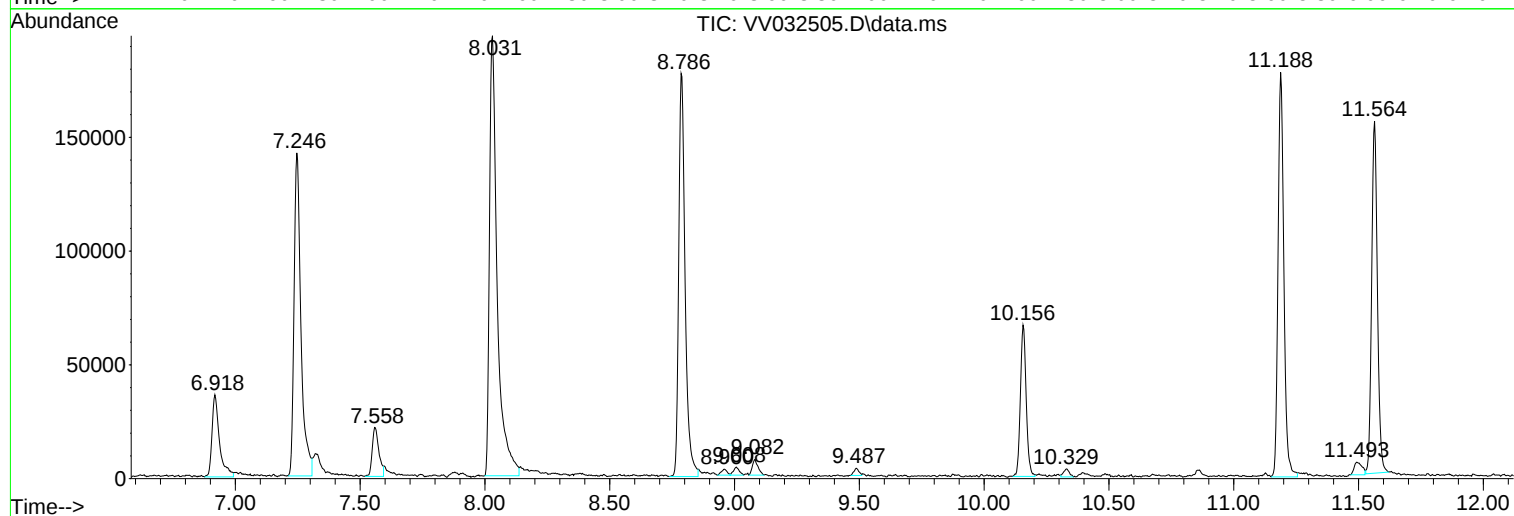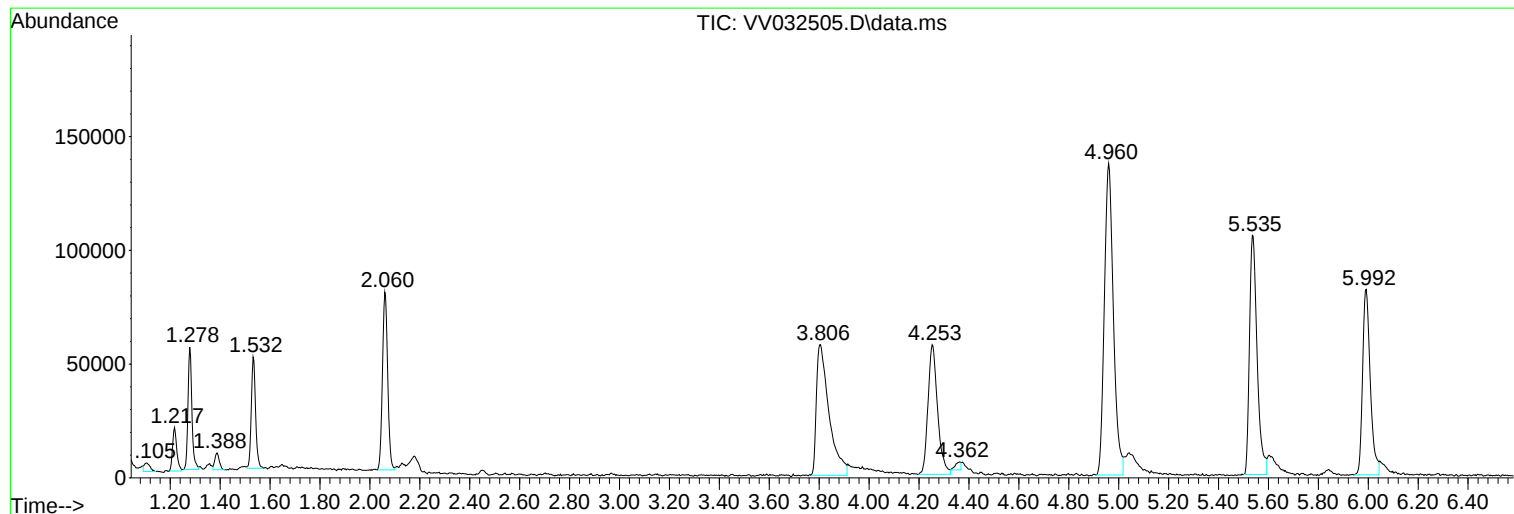

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032505.D
Acq On : 19 Oct 2023 18:30
Operator : SY/MD
Sample : 04950-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49M0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032505.D
Acq On : 19 Oct 2023 18:30
Operator : SY/MD
Sample : 04950-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49M0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc