


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101923\
Data File : VV032484.D
Acq On : 19 Oct 2023 08:25
Operator : SY/MD
Sample : BFB223
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB223

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Oct 21 02:44:24 2023

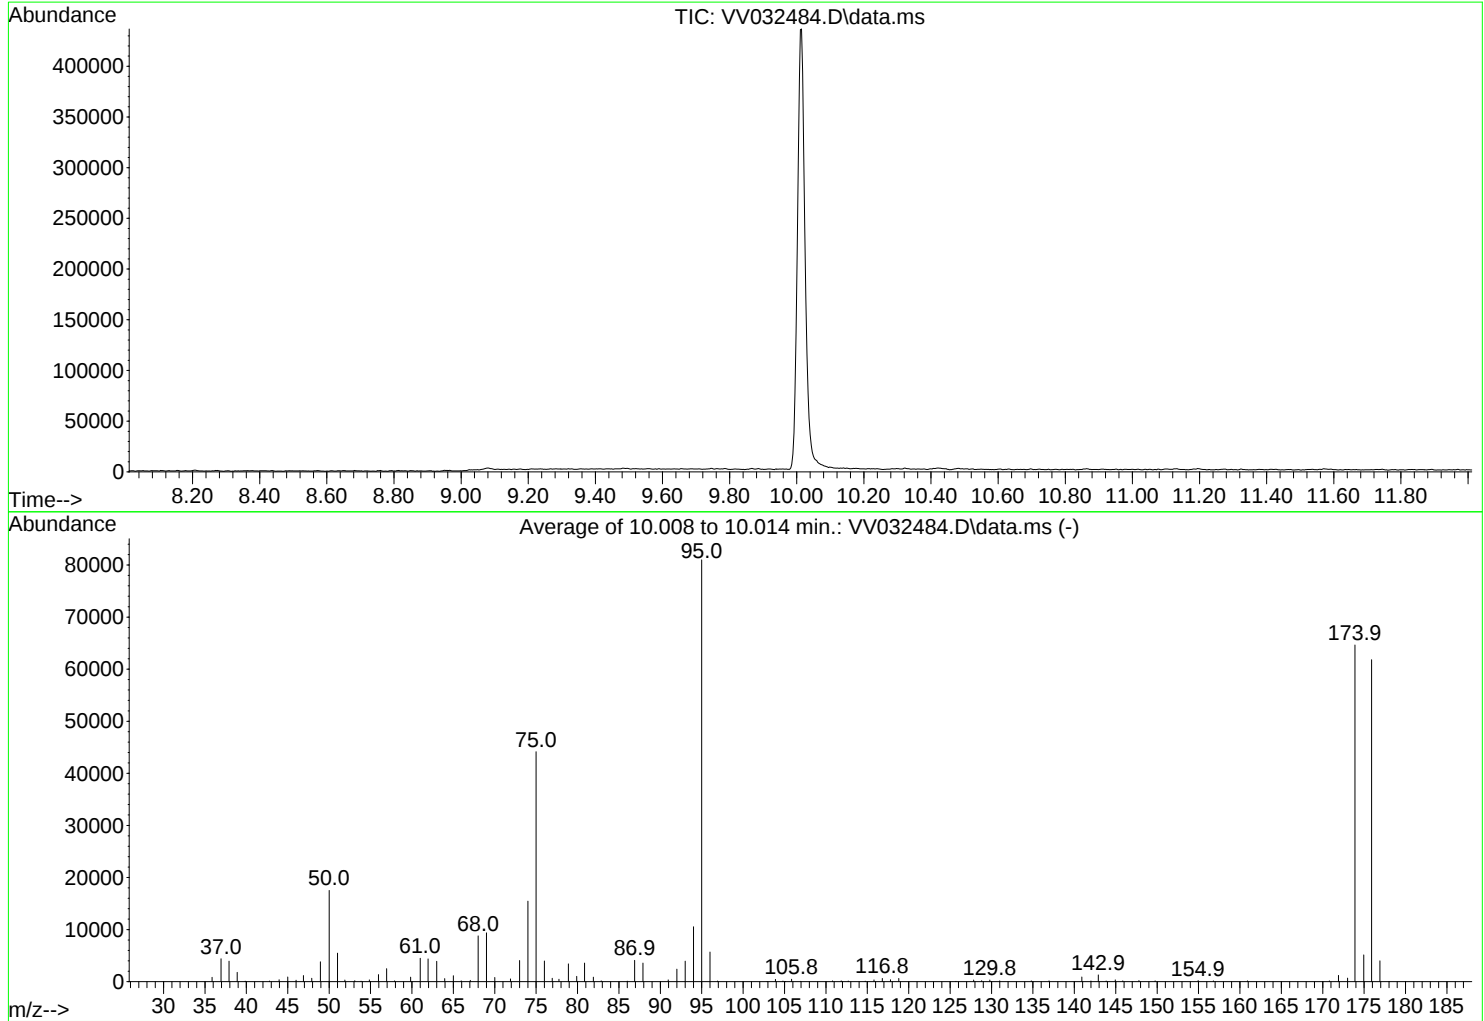

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	17531	PASS
75	95	30	80	54.5	44155	PASS
95	95	100	100	100.0	80997	PASS
96	95	5	9	7.0	5697	PASS
173	174	0.00	2	1.1	689	PASS
174	95	50	120	79.8	64645	PASS
175	174	5	9	7.9	5121	PASS
176	174	95	105	95.6	61829	PASS
177	176	5	10	6.5	4007	PASS

m/z	Abundance
35.90	1360.0
37.10	158.0
37.90	442.0
39.10	103.0
39.80	216.0
40.90	122.0
44.00	379.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
35.90	2240.0
37.00	4405.0
38.00	4040.0
38.90	1734.0
39.90	324.0
41.10	104.0
42.80	152.0
43.90	721.0
45.00	845.0
46.00	241.0
46.90	1092.0
47.90	614.0
48.90	3801.0
50.00	16800.0
51.00	5030.0
51.90	307.0
53.10	184.0
53.90	149.0
54.90	313.0
56.00	1304.0
56.90	2375.0
57.90	162.0
59.90	826.0
61.00	4144.0
62.00	4125.0
63.00	3522.0
63.90	543.0
65.00	958.0
65.90	141.0
67.00	252.0
68.00	8309.0
69.00	8909.0
70.00	770.0
71.90	493.0
73.00	3688.0
74.00	14517.0
75.00	40824.0
76.00	3754.0
76.90	624.0
77.80	412.0
78.90	3251.0
79.90	951.0
80.90	3361.0
81.90	789.0
82.80	172.0
86.90	3761.0
87.90	3332.0
91.00	312.0
92.00	2263.0
93.00	3613.0
94.00	9850.0
95.00	74976.0
96.00	5553.0
96.90	121.0
103.90	376.0
104.80	139.0
105.80	400.0
107.00	111.0
110.70	130.0
111.90	133.0
112.70	103.0
114.70	125.0
115.80	325.0
116.80	587.0
117.80	407.0
118.80	628.0
125.70	101.0
127.80	287.0
128.80	200.0
129.80	280.0
131.00	190.0
134.80	144.0
136.90	151.0
140.90	844.0
142.00	114.0
142.90	1093.0
143.90	117.0
145.00	327.0
145.80	146.0
147.80	215.0
149.80	140.0
155.00	193.0
156.80	137.0
160.90	103.0
170.80	130.0
171.90	1032.0
173.00	973.0
173.90	57896.0
174.90	4800.0
175.90	55336.0
176.90	3735.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
35.90	2265.0
37.00	4660.0
37.90	4447.0
38.90	1919.0
39.90	319.0
41.10	110.0
42.80	136.0
43.90	750.0
45.00	926.0
46.00	296.0
46.90	1208.0
47.90	692.0
48.90	3866.0
50.00	18136.0
51.00	5673.0
51.90	324.0
53.10	185.0
53.80	121.0
54.90	355.0
55.90	1393.0
56.90	2559.0
57.90	169.0
59.90	898.0
61.00	4671.0
62.00	4540.0
63.00	4106.0
63.90	602.0
65.00	1171.0
65.90	162.0
67.10	264.0
68.00	9074.0
69.00	9667.0
70.00	855.0
71.90	555.0
73.00	4155.0
74.00	16024.0
75.00	45944.0
76.00	4104.0
77.00	693.0
77.70	487.0
78.90	3523.0
79.90	1040.0
80.80	3706.0
81.90	916.0
82.90	139.0
86.00	159.0
86.90	4208.0
87.90	3666.0
90.90	355.0
92.00	2459.0
93.00	4119.0
94.00	10892.0
95.00	84056.0
96.00	5885.0
96.90	141.0
103.90	465.0
104.80	141.0
105.80	479.0
106.90	103.0
110.80	146.0
111.90	156.0
112.70	118.0
114.80	118.0
115.80	338.0
116.80	645.0
117.80	386.0
118.80	664.0
125.70	103.0
127.80	304.0
128.80	181.0
129.80	329.0
131.00	169.0
134.80	162.0
137.00	164.0
140.90	928.0
142.00	136.0
142.90	1358.0
143.80	126.0
145.00	362.0
145.90	163.0
147.80	223.0
149.80	151.0
154.90	231.0
156.80	166.0
160.90	156.0
170.80	152.0
171.90	1265.0
173.00	1094.0
173.90	67048.0
174.90	5300.0
175.90	64216.0
176.90	4135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
35.90	2070.0
36.90	4632.0
37.90	4609.0
38.90	2013.0
39.90	325.0
40.90	112.0
42.80	127.0
44.00	757.0
45.00	895.0
46.00	290.0
46.90	1202.0
47.90	674.0
49.00	3742.0
50.00	17656.0
51.00	5698.0
51.90	327.0
53.10	162.0
54.80	356.0
55.90	1342.0
57.00	2535.0
57.90	182.0
59.80	900.0
61.00	4637.0
61.90	4435.0
63.00	4125.0
64.00	635.0
65.00	1293.0
66.00	168.0
67.10	260.0
68.00	8950.0
69.00	9541.0
70.00	821.0
71.90	521.0
73.00	4340.0
74.00	15782.0
75.00	45696.0
76.00	3998.0
77.00	630.0
77.70	509.0
78.90	3416.0
79.90	1042.0
80.80	3660.0
81.90	917.0
82.90	134.0
86.00	167.0
86.90	4334.0
87.90	3682.0
90.90	381.0
92.00	2490.0
93.00	4051.0
94.00	10913.0
95.00	83960.0
96.00	5653.0
96.90	148.0
102.90	103.0
103.90	475.0
104.80	122.0
105.10	117.0
105.90	502.0
110.90	177.0
111.80	140.0
112.70	122.0
115.80	334.0
116.80	641.0
117.80	318.0
118.80	570.0
127.90	312.0
128.80	150.0
129.80	307.0
131.00	123.0
134.80	170.0
137.00	148.0
140.90	882.0
142.00	147.0
142.90	1429.0
143.80	136.0
144.90	318.0
145.90	161.0
147.80	211.0
149.70	153.0
154.90	231.0
156.80	191.0
160.90	168.0
170.80	171.0
171.90	1341.0
173.90	68992.0
175.00	5263.0
175.90	65936.0
176.90	4151.0
178.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223