

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019007.D
 Acq On : 20 Oct 2020 12:26
 Operator : SY/MD
 Sample : L4382-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	85	rVB	131574	133079	16.44%	2.293%
2	1.579	145	152	165	rVB	102851	117827	14.55%	2.030%
3	2.122	312	321	345	rVB	207874	318659	39.36%	5.491%
4	2.672	490	492	494	rBV2	492	221	0.03%	0.004%
5	2.907	561	565	567	rBV	539	446	0.06%	0.008%
6	3.071	612	616	621	rBV2	611	644	0.08%	0.011%
7	3.267	670	677	682	rBV3	687	1007	0.12%	0.017%
8	3.560	765	768	770	rBV2	485	281	0.03%	0.005%
9	3.643	793	794	795	rBV	352	120	0.01%	0.002%
10	3.685	805	807	809	rBV2	419	235	0.03%	0.004%
11	3.862	861	862	867	rBV2	287	199	0.02%	0.003%
12	3.916	869	879	914	rBV2	53025	164637	20.34%	2.837%
13	4.376	1008	1022	1046	rBV	126973	317560	39.23%	5.472%
14	4.682	1111	1117	1120	rBV3	486	530	0.07%	0.009%
15	4.707	1123	1125	1129	rVV3	652	438	0.05%	0.008%
16	5.006	1216	1218	1221	rBV	487	257	0.03%	0.004%
17	5.074	1222	1239	1268	rVV2	315239	809584	100.00%	13.950%
18	5.505	1371	1373	1375	rBV3	463	257	0.03%	0.004%
19	5.643	1404	1416	1440	rBV	252571	509799	62.97%	8.785%
20	5.859	1481	1483	1484	rBV	384	143	0.02%	0.002%
21	5.929	1493	1505	1524	rBV2	31121	66061	8.16%	1.138%
22	6.093	1544	1556	1589	rBV	161608	330419	40.81%	5.694%
23	6.293	1616	1618	1621	rVB2	209	106	0.01%	0.002%
24	6.334	1628	1631	1632	rBV	254	152	0.02%	0.003%
25	6.399	1648	1651	1654	rVB2	337	200	0.02%	0.003%
26	6.415	1654	1656	1659	rBV2	216	114	0.01%	0.002%
27	6.463	1667	1671	1674	rBV	210	164	0.02%	0.003%
28	6.492	1678	1680	1684	rVB	388	222	0.03%	0.004%
29	6.563	1699	1702	1707	rBB2	121	116	0.01%	0.002%
30	6.588	1707	1710	1713	rBV	213	137	0.02%	0.002%
31	6.627	1716	1722	1725	rBV	429	482	0.06%	0.008%
32	6.669	1732	1735	1737	rBV	262	126	0.02%	0.002%
33	6.694	1738	1743	1745	rBV3	389	297	0.04%	0.005%
34	6.743	1755	1758	1760	rBV	318	221	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019007.D
 Acq On : 20 Oct 2020 12:26
 Operator : SY/MD
 Sample : L4382-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.785	1768	1771	1773	rBV2	274	185	0.02%	0.003%
36	6.801	1774	1776	1779	rVB	335	144	0.02%	0.002%
37	6.961	1825	1826	1830	rVB	129	36	0.00%	0.001%
38	7.010	1830	1841	1866	rBV	84806	158685	19.60%	2.734%
39	7.338	1931	1943	1972	rBV	319192	555439	68.61%	9.571%
40	7.592	2020	2022	2023	rBV	244	130	0.02%	0.002%
41	7.643	2029	2038	2059	rBV	59664	107085	13.23%	1.845%
42	7.903	2116	2119	2122	rBV4	391	346	0.04%	0.006%
43	7.958	2132	2136	2140	rBV3	438	509	0.06%	0.009%
44	8.000	2143	2149	2154	rBV5	1786	2087	0.26%	0.036%
45	8.032	2156	2159	2164	rVB	587	416	0.05%	0.007%
46	8.058	2164	2167	2169	rVB	233	117	0.01%	0.002%
47	8.074	2169	2172	2174	rBV2	304	156	0.02%	0.003%
48	8.109	2174	2183	2218	rBV2	133500	293327	36.23%	5.055%
49	8.505	2305	2306	2307	rBV	169	52	0.01%	0.001%
50	8.514	2307	2309	2313	rVV2	344	226	0.03%	0.004%
51	8.595	2330	2334	2335	rBV2	308	203	0.03%	0.003%
52	8.653	2351	2352	2356	rVB	313	136	0.02%	0.002%
53	8.746	2378	2381	2382	rBV	330	144	0.02%	0.002%
54	8.874	2409	2421	2449	rBV	364517	600229	74.14%	10.343%
55	9.186	2514	2518	2522	rBV	280	275	0.03%	0.005%
56	9.209	2522	2525	2530	rVV2	221	177	0.02%	0.003%
57	9.399	2581	2584	2586	rBV	361	238	0.03%	0.004%
58	9.463	2600	2604	2607	rBV	348	313	0.04%	0.005%
59	9.508	2614	2618	2619	rBV	248	156	0.02%	0.003%
60	9.543	2627	2629	2630	rBV	179	57	0.01%	0.001%
61	9.624	2649	2654	2658	rBV2	350	417	0.05%	0.007%
62	9.772	2695	2700	2702	rBV2	377	261	0.03%	0.004%
63	9.788	2702	2705	2708	rBV2	408	273	0.03%	0.005%
64	9.836	2715	2720	2722	rBV2	259	262	0.03%	0.005%
65	9.974	2761	2763	2764	rBV2	177	89	0.01%	0.002%
66	9.984	2764	2766	2772	rVB2	405	332	0.04%	0.006%
67	10.074	2791	2794	2797	rBV	223	175	0.02%	0.003%
68	10.238	2833	2845	2869	rBV	156184	249138	30.77%	4.293%
69	10.659	2973	2976	2979	rBV2	332	288	0.04%	0.005%
70	10.714	2991	2993	2996	rBV	218	128	0.02%	0.002%
71	10.800	3017	3020	3022	rBV2	285	168	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019007.D
 Acq On : 20 Oct 2020 12:26
 Operator : SY/MD
 Sample : L4382-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	11.013	3084	3086	3087	rBV	166	49	0.01%	0.001%
73	11.170	3131	3135	3137	rBV2	247	189	0.02%	0.003%
74	11.270	3155	3166	3185	rBV	344717	543869	67.18%	9.372%
75	11.579	3258	3262	3265	rVB	359	256	0.03%	0.004%
76	11.646	3271	3283	3301	rBV	318292	509360	62.92%	8.777%
77	11.968	3379	3383	3387	rBV3	459	438	0.05%	0.008%
78	12.103	3423	3425	3427	rBV2	308	145	0.02%	0.002%
79	12.148	3435	3439	3441	rBV	374	319	0.04%	0.005%
80	12.222	3460	3462	3468	rBV	336	337	0.04%	0.006%
81	12.884	3666	3668	3671	rVB2	347	147	0.02%	0.003%
82	13.045	3716	3718	3722	rBV2	268	185	0.02%	0.003%
83	13.067	3722	3725	3726	rBV2	382	256	0.03%	0.004%
84	13.614	3893	3895	3898	rBV	236	149	0.02%	0.003%
85	13.672	3911	3913	3914	rBV	385	174	0.02%	0.003%
86	13.861	3969	3972	3974	rBV2	461	260	0.03%	0.004%


Sum of corrected areas: 5803272

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102020\
Data File : VV019007.D
Acq On : 20 Oct 2020 12:26
Operator : SY/MD
Sample : L4382-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

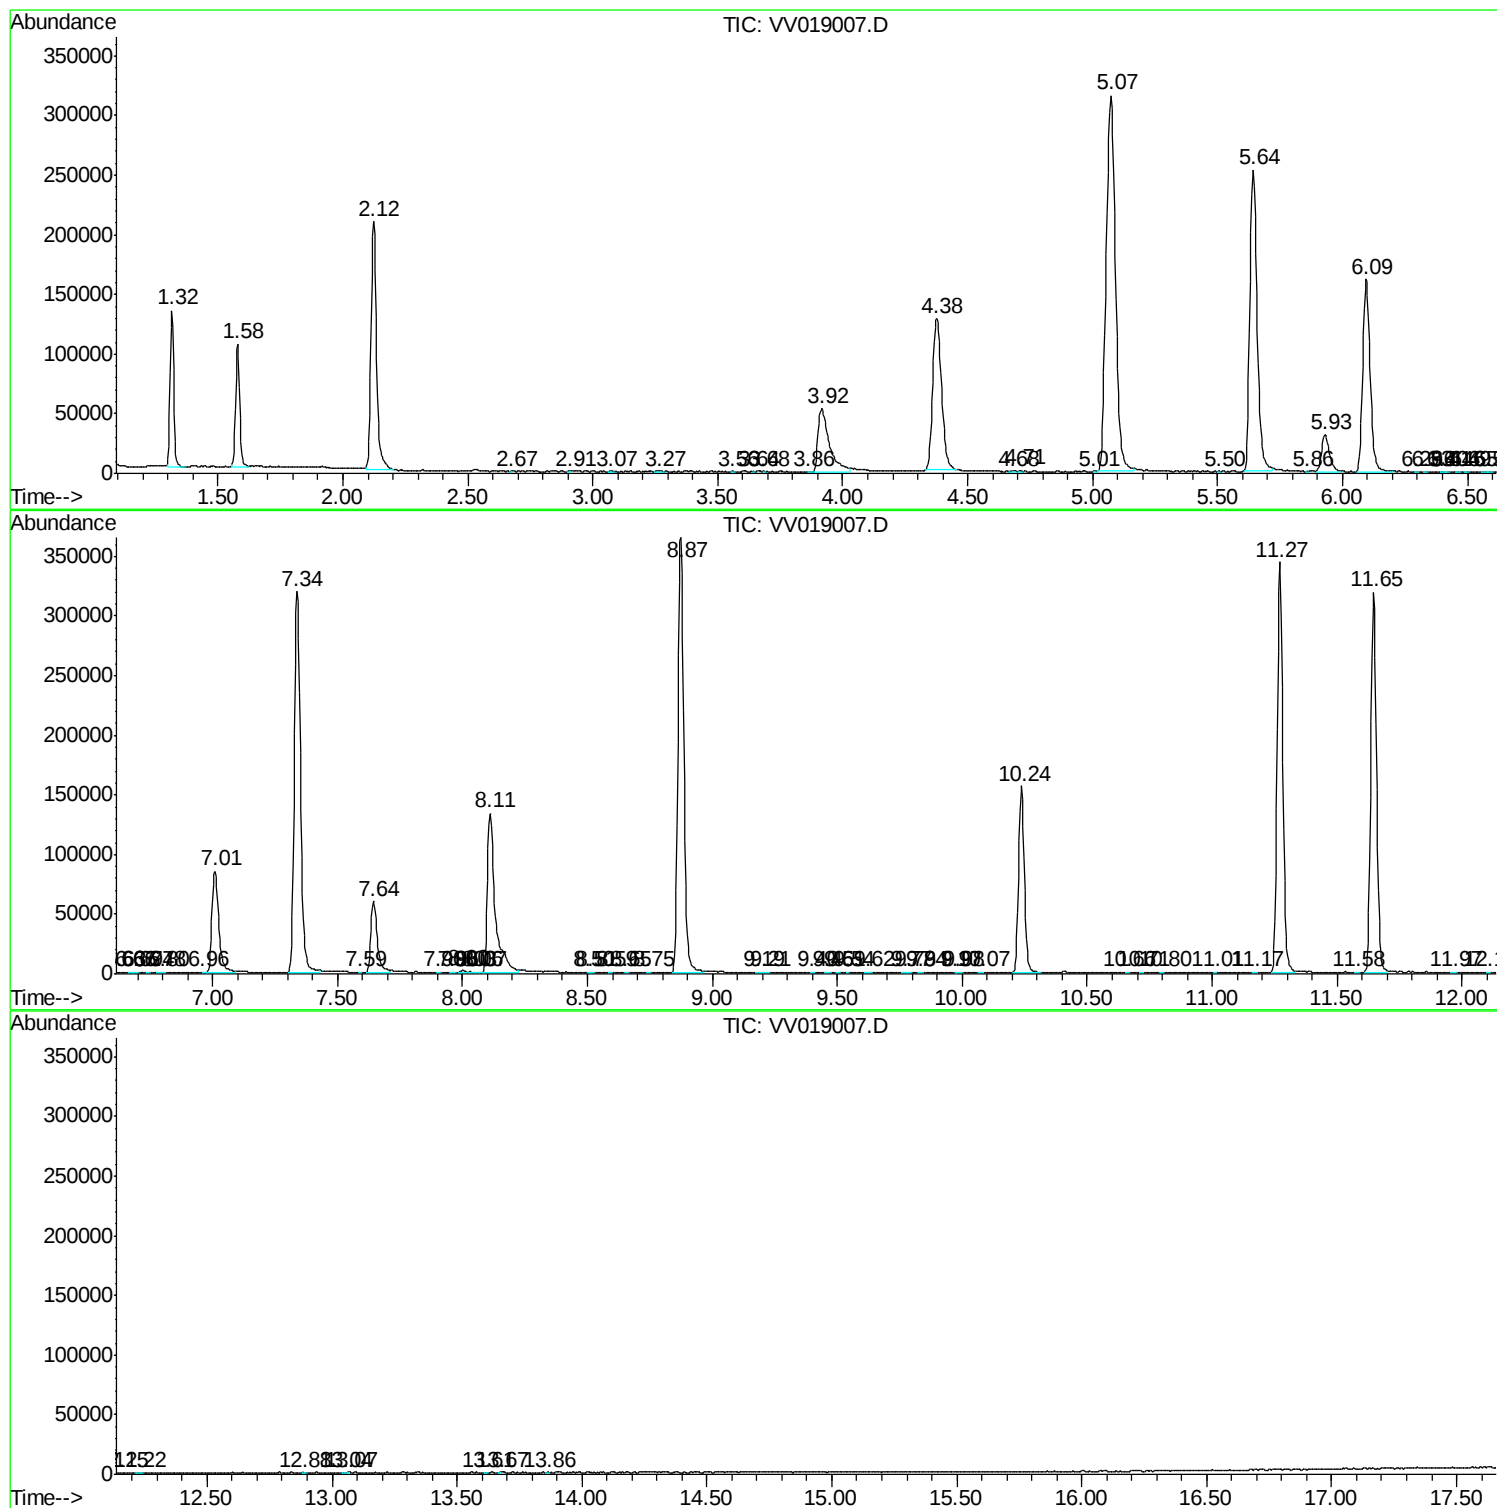

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102020\
Data File : VV019007.D
Acq On : 20 Oct 2020 12:26
Operator : SY/MD
Sample : L4382-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102020\
Data File : VV019007.D
Acq On : 20 Oct 2020 12:26
Operator : SY/MD
Sample : L4382-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc