

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019011.D
 Acq On : 20 Oct 2020 14:00
 Operator : SY/MD
 Sample : L4430-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	122451	124285	10.87%	1.378%
2	1.579	145	152	162	rBV	125580	143144	12.52%	1.587%
3	2.122	312	321	358	rVB	247179	394512	34.49%	4.374%
4	2.888	557	559	564	rVB3	479	367	0.03%	0.004%
5	2.949	575	578	579	rBV	342	197	0.02%	0.002%
6	3.158	638	643	645	rBV	262	276	0.02%	0.003%
7	3.180	648	650	654	rVV2	314	185	0.02%	0.002%
8	3.229	661	665	672	rVB4	620	639	0.06%	0.007%
9	3.303	684	688	690	rBV	312	211	0.02%	0.002%
10	3.354	701	704	705	rBV	258	140	0.01%	0.002%
11	3.608	780	783	788	rBV	372	292	0.03%	0.003%
12	3.727	816	820	823	rBV3	537	467	0.04%	0.005%
13	3.843	854	856	857	rBV	139	70	0.01%	0.001%
14	3.917	866	879	917	rBV	87613	285031	24.92%	3.160%
15	4.376	1007	1022	1050	rBV	189043	460551	40.27%	5.106%
16	4.849	1167	1169	1170	rBV	265	94	0.01%	0.001%
17	4.929	1192	1194	1195	rBV	227	95	0.01%	0.001%
18	4.942	1195	1198	1200	rVB	308	166	0.01%	0.002%
19	4.958	1200	1203	1204	rBV	373	172	0.02%	0.002%
20	5.071	1222	1238	1268	rBV2	442671	1143775	100.00%	12.680%
21	5.309	1309	1312	1315	rBV5	599	468	0.04%	0.005%
22	5.328	1315	1318	1319	rBV	298	171	0.01%	0.002%
23	5.409	1341	1343	1346	rBV2	328	152	0.01%	0.002%
24	5.527	1378	1380	1383	rBV	352	197	0.02%	0.002%
25	5.589	1396	1399	1401	rBV3	356	284	0.02%	0.003%
26	5.640	1404	1415	1449	rVV	371015	751704	65.72%	8.333%
27	5.827	1470	1473	1479	rVB4	692	621	0.05%	0.007%
28	5.878	1486	1489	1491	rBV3	504	321	0.03%	0.004%
29	5.933	1494	1506	1532	rVB5	36341	85170	7.45%	0.944%
30	6.093	1543	1556	1588	rBV	265108	545812	47.72%	6.051%
31	6.318	1623	1626	1628	rVB	475	313	0.03%	0.003%
32	6.331	1628	1630	1633	rBV	230	124	0.01%	0.001%
33	6.347	1633	1635	1637	rBV2	631	367	0.03%	0.004%
34	6.518	1684	1688	1690	rBV3	520	411	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019011.D
 Acq On : 20 Oct 2020 14:00
 Operator : SY/MD
 Sample : L4430-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.582	1705	1708	1713	rBV3	553	534	0.05%	0.006%
36	6.666	1726	1734	1736	rBV4	1042	1195	0.10%	0.013%
37	6.788	1770	1772	1775	rBV	539	355	0.03%	0.004%
38	6.823	1781	1783	1786	rBV	381	249	0.02%	0.003%
39	6.875	1796	1799	1801	rVB	264	129	0.01%	0.001%
40	6.913	1809	1811	1815	rBV	559	318	0.03%	0.004%
41	7.010	1829	1841	1861	rBV	126750	233826	20.44%	2.592%
42	7.338	1930	1943	1967	rBV	491116	860689	75.25%	9.541%
43	7.643	2028	2038	2059	rBV	91770	160675	14.05%	1.781%
44	7.881	2109	2112	2115	rVB	435	304	0.03%	0.003%
45	7.923	2115	2125	2129	rBV2	494	967	0.08%	0.011%
46	7.955	2131	2135	2137	rBV3	664	585	0.05%	0.006%
47	8.000	2143	2149	2164	rVB7	7517	12726	1.11%	0.141%
48	8.109	2170	2183	2226	rBV2	268028	580518	50.75%	6.436%
49	8.534	2312	2315	2317	rBV2	411	241	0.02%	0.003%
50	8.627	2341	2344	2345	rBV2	441	248	0.02%	0.003%
51	8.653	2350	2352	2356	rVB	662	373	0.03%	0.004%
52	8.707	2365	2369	2373	rBV2	420	304	0.03%	0.003%
53	8.733	2373	2377	2379	rBV2	307	291	0.03%	0.003%
54	8.756	2381	2384	2385	rBV	365	209	0.02%	0.002%
55	8.804	2395	2399	2402	rBV2	430	386	0.03%	0.004%
56	8.820	2402	2404	2408	rVB	393	208	0.02%	0.002%
57	8.875	2408	2421	2442	rBV	589284	957233	83.69%	10.612%
58	9.077	2482	2484	2487	rBV	480	256	0.02%	0.003%
59	9.145	2502	2505	2507	rBV	422	251	0.02%	0.003%
60	9.206	2522	2524	2527	rVB3	413	195	0.02%	0.002%
61	9.222	2527	2529	2532	rBV3	223	125	0.01%	0.001%
62	9.302	2552	2554	2556	rVB	484	190	0.02%	0.002%
63	9.322	2556	2560	2564	rBV2	306	319	0.03%	0.004%
64	9.441	2594	2597	2599	rBV2	320	260	0.02%	0.003%
65	9.540	2625	2628	2629	rBV2	412	207	0.02%	0.002%
66	9.598	2644	2646	2648	rBV	436	247	0.02%	0.003%
67	9.656	2661	2664	2668	rVB	376	299	0.03%	0.003%
68	9.688	2670	2674	2675	rBV	342	207	0.02%	0.002%
69	9.785	2702	2704	2706	rBV	300	142	0.01%	0.002%
70	9.817	2711	2714	2715	rBV	245	138	0.01%	0.002%
71	9.907	2740	2742	2746	rVB	298	168	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019011.D
 Acq On : 20 Oct 2020 14:00
 Operator : SY/MD
 Sample : L4430-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	9.945	2750	2754	2760	rBV3	490	433	0.04%	0.005%
73	9.974	2760	2763	2764	rBV2	433	264	0.02%	0.003%
74	10.032	2778	2781	2788	rVB4	541	485	0.04%	0.005%
75	10.103	2801	2803	2807	rVB2	232	100	0.01%	0.001%
76	10.235	2833	2844	2869	rBV	325144	510907	44.67%	5.664%
77	10.399	2890	2895	2896	rBV5	1429	1149	0.10%	0.013%
78	10.508	2924	2929	2931	rBV3	508	425	0.04%	0.005%
79	10.624	2963	2965	2968	rVB2	503	244	0.02%	0.003%
80	10.926	3055	3059	3064	rBV3	431	428	0.04%	0.005%
81	11.270	3154	3166	3191	rBV	564597	879920	76.93%	9.755%
82	11.550	3249	3253	3257	rBV2	411	426	0.04%	0.005%
83	11.646	3268	3283	3305	rBV	561486	867899	75.88%	9.621%
84	12.598	3575	3579	3584	rBV3	625	656	0.06%	0.007%
85	12.784	3635	3637	3644	rBV2	493	508	0.04%	0.006%
86	13.746	3933	3936	3938	rBV2	491	287	0.03%	0.003%


Sum of corrected areas: 9020482

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102020\
Data File : VV019011.D
Acq On : 20 Oct 2020 14:00
Operator : SY/MD
Sample : L4430-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

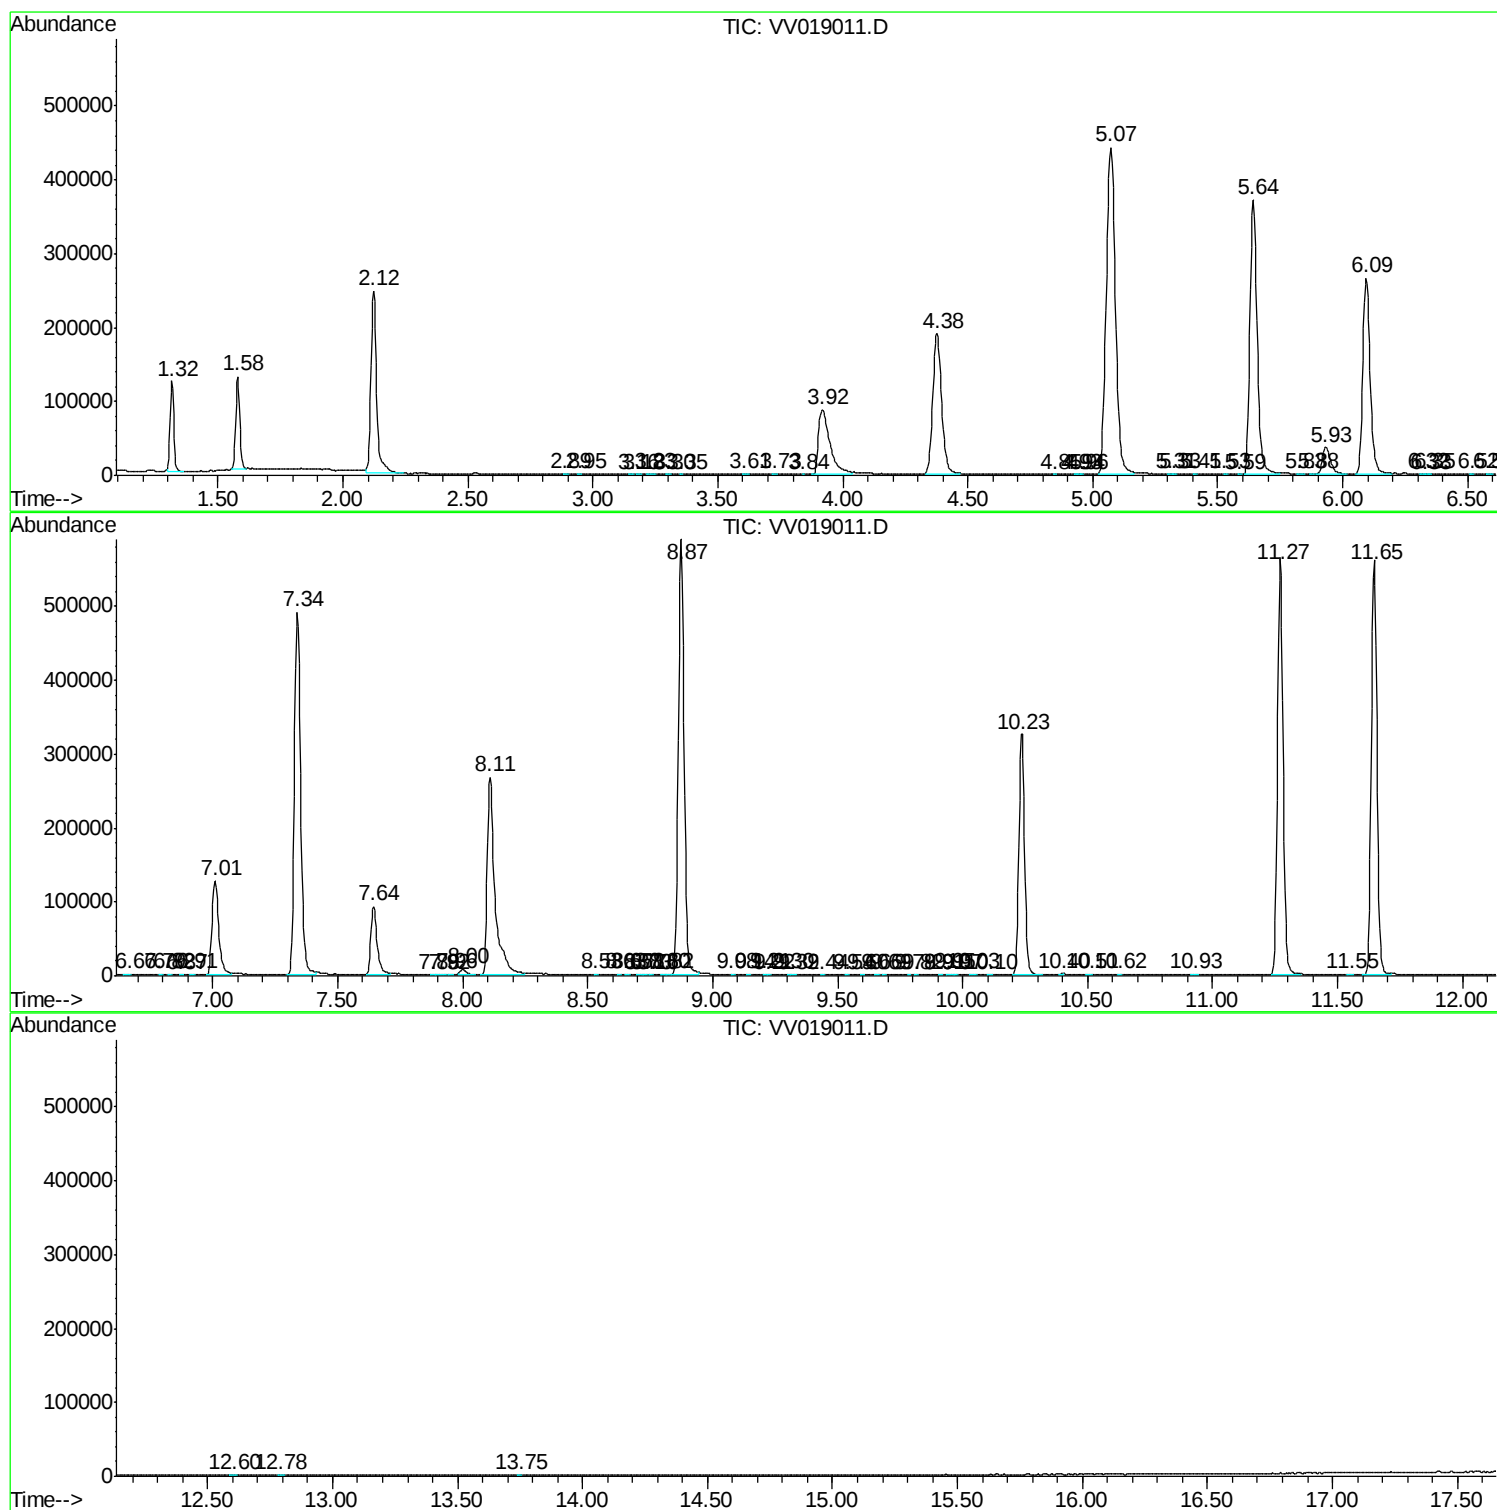

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102020\
Data File : VV019011.D
Acq On : 20 Oct 2020 14:00
Operator : SY/MD
Sample : L4430-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102020\
Data File : VV019011.D
Acq On : 20 Oct 2020 14:00
Operator : SY/MD
Sample : L4430-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc