

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019017.D
 Acq On : 20 Oct 2020 16:22
 Operator : SY/MD
 Sample : L4430-01DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	84	rVB2	179085	190920	18.13%	2.005%
2	1.576	145	151	163	rBV	127672	143717	13.65%	1.510%
3	2.119	310	320	347	rVB	243806	387574	36.81%	4.071%
4	3.061	610	613	617	rBV2	798	618	0.06%	0.006%
5	3.200	653	656	658	rBV2	542	386	0.04%	0.004%
6	3.258	672	674	677	rBV	408	177	0.02%	0.002%
7	3.486	743	745	749	rVB	515	311	0.03%	0.003%
8	3.557	764	767	768	rBV	311	150	0.01%	0.002%
9	3.586	774	776	779	rVB2	292	161	0.02%	0.002%
10	3.663	797	800	803	rBV	380	330	0.03%	0.003%
11	3.933	867	884	915	rBV2	319354	924302	87.78%	9.709%
12	4.373	1007	1021	1049	rVB	182121	455468	43.26%	4.784%
13	4.685	1116	1118	1123	rBV2	484	392	0.04%	0.004%
14	4.788	1147	1150	1151	rBV	197	115	0.01%	0.001%
15	4.859	1169	1172	1175	rVB2	397	258	0.02%	0.003%
16	4.885	1175	1180	1183	rBV2	351	286	0.03%	0.003%
17	4.923	1189	1192	1195	rBV2	359	326	0.03%	0.003%
18	4.949	1198	1200	1203	rVB	543	255	0.02%	0.003%
19	4.978	1203	1209	1212	rBV2	292	284	0.03%	0.003%
20	5.003	1212	1217	1220	rBV2	444	389	0.04%	0.004%
21	5.071	1220	1238	1272	rBV2	407486	1052964	100.00%	11.060%
22	5.261	1296	1297	1299	rBV2	531	230	0.02%	0.002%
23	5.293	1304	1307	1311	rBV3	566	430	0.04%	0.005%
24	5.331	1316	1319	1321	rBV	203	110	0.01%	0.001%
25	5.364	1321	1329	1330	rBV2	840	918	0.09%	0.010%
26	5.441	1351	1353	1356	rVB	300	143	0.01%	0.002%
27	5.466	1360	1361	1363	rBV	304	86	0.01%	0.001%
28	5.499	1369	1371	1373	rBV	235	81	0.01%	0.001%
29	5.547	1383	1386	1388	rBV	222	110	0.01%	0.001%
30	5.573	1388	1394	1400	rBV3	384	460	0.04%	0.005%
31	5.640	1400	1415	1437	rBV	384205	756083	71.81%	7.942%
32	5.930	1492	1505	1527	rBV4	50486	117763	11.18%	1.237%
33	6.093	1542	1556	1584	rBV	244876	498301	47.32%	5.234%
34	6.306	1619	1622	1624	rBV2	399	249	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019017.D
 Acq On : 20 Oct 2020 16:22
 Operator : SY/MD
 Sample : L4430-01DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.367	1637	1641	1646	rVB2	245	212	0.02%	0.002%
36	6.393	1646	1649	1650	rBV	221	115	0.01%	0.001%
37	6.418	1655	1657	1660	rVB2	200	108	0.01%	0.001%
38	6.434	1660	1662	1666	rVB2	384	229	0.02%	0.002%
39	6.457	1666	1669	1671	rBV	251	162	0.02%	0.002%
40	6.499	1679	1682	1683	rBV2	228	110	0.01%	0.001%
41	6.624	1717	1721	1723	rBV2	230	174	0.02%	0.002%
42	6.778	1767	1769	1773	rVB3	289	161	0.02%	0.002%
43	6.820	1775	1782	1783	rBV2	252	241	0.02%	0.003%
44	6.830	1783	1785	1790	rVB	405	280	0.03%	0.003%
45	6.856	1790	1793	1796	rBV2	264	228	0.02%	0.002%
46	6.891	1801	1804	1808	rBV2	341	226	0.02%	0.002%
47	7.007	1829	1840	1863	rBV	124528	227860	21.64%	2.393%
48	7.338	1931	1943	1964	rBV	458371	791130	75.13%	8.310%
49	7.556	2010	2011	2012	rBV	285	101	0.01%	0.001%
50	7.643	2024	2038	2068	rBV	90996	163703	15.55%	1.720%
51	7.907	2116	2120	2124	rBV3	325	264	0.03%	0.003%
52	7.933	2124	2128	2130	rBV2	376	321	0.03%	0.003%
53	7.997	2139	2148	2169	rVB2	37123	64755	6.15%	0.680%
54	8.113	2173	2184	2227	rBV2	238387	554106	52.62%	5.820%
55	8.508	2305	2307	2308	rBV	310	154	0.01%	0.002%
56	8.621	2338	2342	2344	rBV3	529	335	0.03%	0.004%
57	8.724	2371	2374	2376	rBV2	450	201	0.02%	0.002%
58	8.736	2376	2378	2380	rBV3	318	171	0.02%	0.002%
59	8.775	2387	2390	2391	rBV	301	174	0.02%	0.002%
60	8.794	2394	2396	2400	rVV	301	187	0.02%	0.002%
61	8.871	2408	2420	2443	rBV	590818	956815	90.87%	10.050%
62	9.161	2507	2510	2513	rBV4	924	648	0.06%	0.007%
63	9.212	2523	2526	2530	rVB	500	386	0.04%	0.004%
64	9.238	2530	2534	2537	rBV2	497	369	0.04%	0.004%
65	9.286	2547	2549	2552	rVB	214	98	0.01%	0.001%
66	9.318	2556	2559	2567	rVB	632	529	0.05%	0.006%
67	9.360	2567	2572	2577	rVB2	431	391	0.04%	0.004%
68	9.389	2577	2581	2582	rBV	363	229	0.02%	0.002%
69	9.402	2583	2585	2593	rVB2	328	227	0.02%	0.002%
70	9.463	2602	2604	2608	rBV	295	209	0.02%	0.002%
71	9.560	2632	2634	2639	rBV3	430	365	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019017.D
 Acq On : 20 Oct 2020 16:22
 Operator : SY/MD
 Sample : L4430-01DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	9.605	2646	2648	2654	rVB2	433	304	0.03%	0.003%
73	9.643	2657	2660	2662	rVB2	270	156	0.01%	0.002%
74	9.659	2662	2665	2670	rBV2	420	314	0.03%	0.003%
75	9.698	2673	2677	2682	rBV	343	268	0.03%	0.003%
76	9.752	2692	2694	2698	rBV3	316	176	0.02%	0.002%
77	9.804	2708	2710	2712	rBV	282	135	0.01%	0.001%
78	9.968	2758	2761	2766	rBV2	319	259	0.02%	0.003%
79	10.010	2771	2774	2777	rBV	259	189	0.02%	0.002%
80	10.148	2814	2817	2820	rBV	281	250	0.02%	0.003%
81	10.238	2833	2845	2866	rBV	282063	451533	42.88%	4.743%
82	10.463	2913	2915	2917	rBV	185	94	0.01%	0.001%
83	10.563	2942	2946	2949	rBV2	235	188	0.02%	0.002%
84	10.736	2998	3000	3002	rBV	234	138	0.01%	0.001%
85	10.842	3029	3033	3035	rBV	525	287	0.03%	0.003%
86	10.994	3077	3080	3084	rBV	337	289	0.03%	0.003%
87	11.032	3091	3092	3093	rBV	174	62	0.01%	0.001%
88	11.077	3103	3106	3109	rBV2	283	234	0.02%	0.002%
89	11.209	3142	3147	3149	rBV2	504	411	0.04%	0.004%
90	11.270	3155	3166	3189	rBV	614172	927312	88.07%	9.740%
91	11.450	3219	3222	3225	rBV4	462	283	0.03%	0.003%
92	11.476	3227	3230	3232	rBV2	411	271	0.03%	0.003%
93	11.511	3239	3241	3246	rBV2	262	301	0.03%	0.003%
94	11.553	3251	3254	3257	rBV2	317	245	0.02%	0.003%
95	11.646	3271	3283	3303	rBV	538075	832369	79.05%	8.743%
96	11.920	3363	3368	3376	rBV7	2321	2744	0.26%	0.029%
97	12.003	3389	3394	3398	rBV2	446	546	0.05%	0.006%
98	12.138	3434	3436	3438	rVB	214	69	0.01%	0.001%
99	12.183	3447	3450	3454	rVB2	306	246	0.02%	0.003%
100	12.206	3454	3457	3459	rBV	389	293	0.03%	0.003%


Sum of corrected areas: 9520287

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102020\
Data File : VV019017.D
Acq On : 20 Oct 2020 16:22
Operator : SY/MD
Sample : L4430-01DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

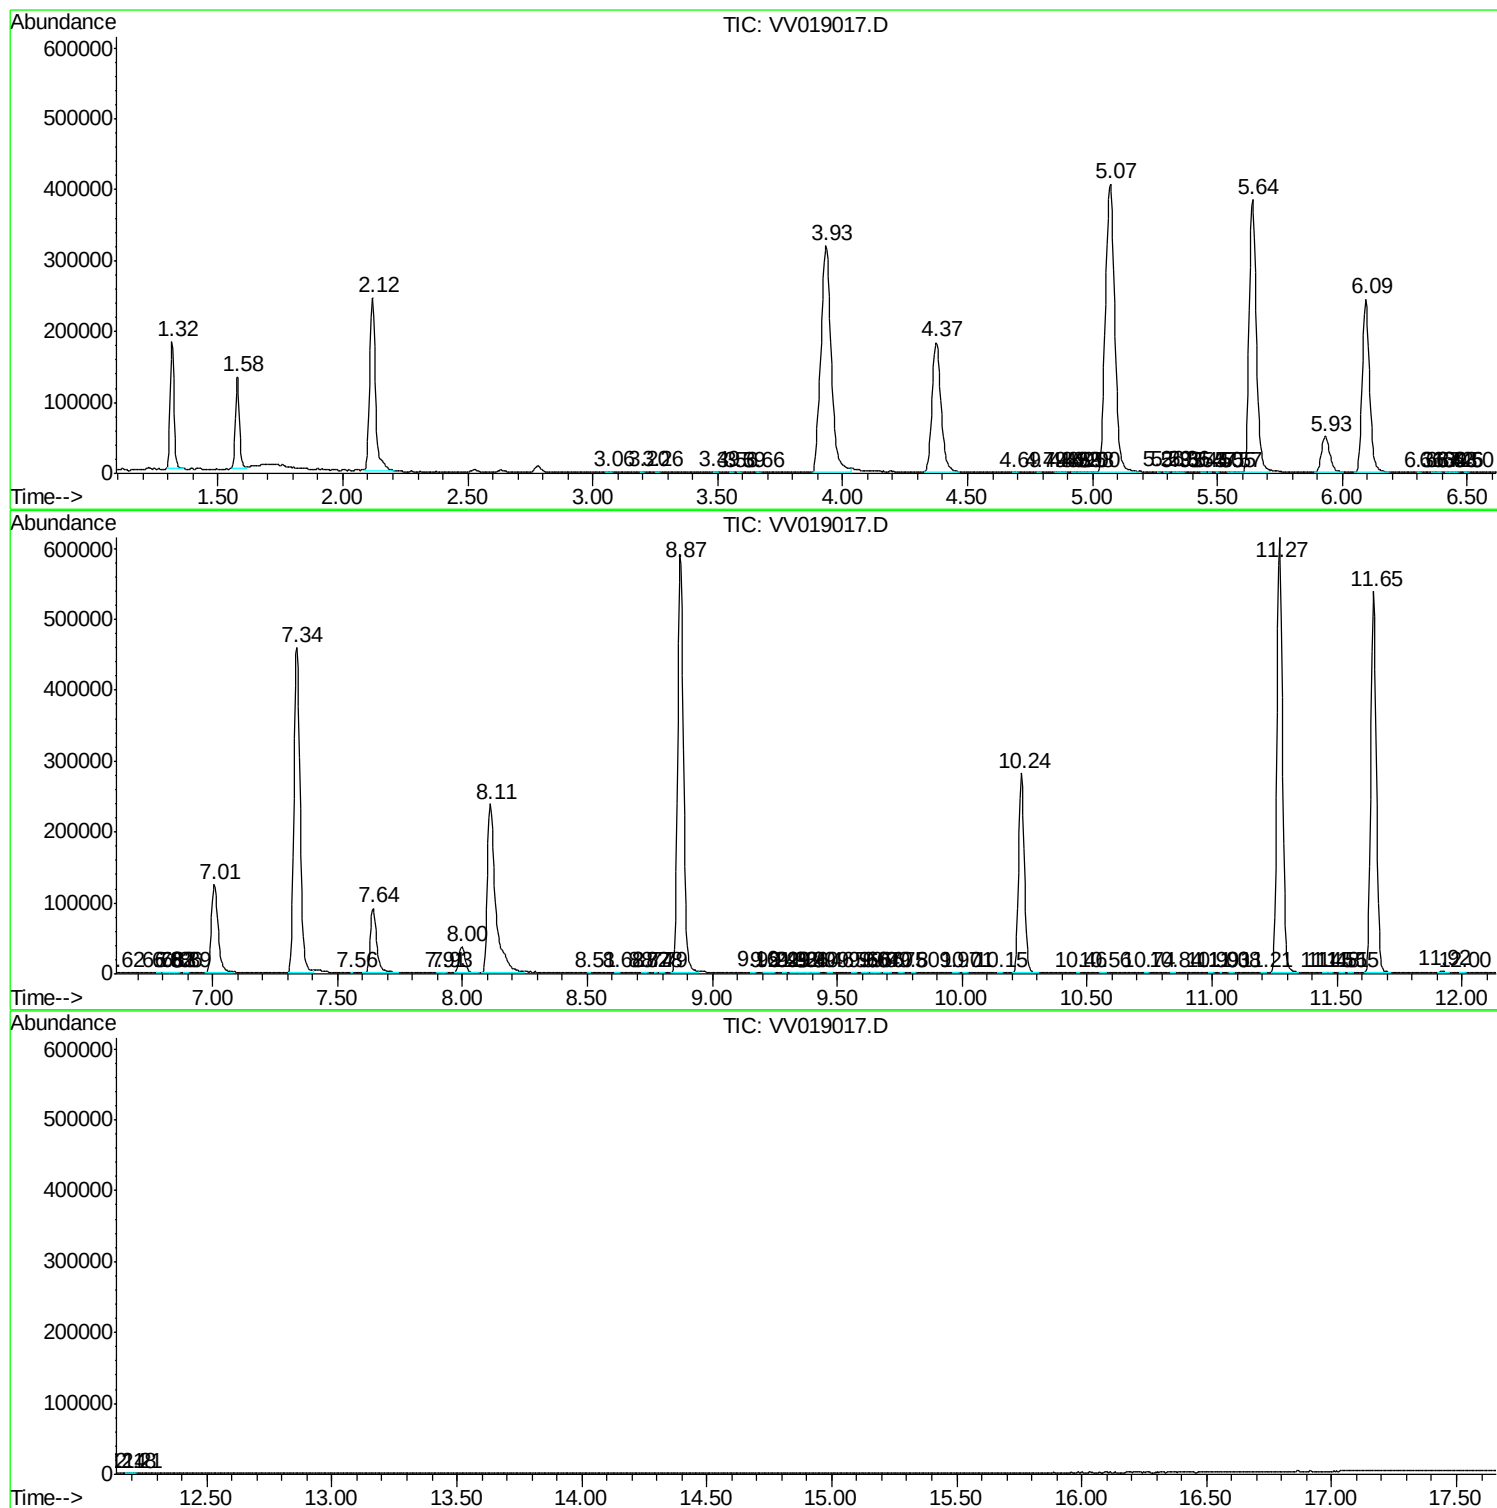

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102020\
Data File : VV019017.D
Acq On : 20 Oct 2020 16:22
Operator : SY/MD
Sample : L4430-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102020\
Data File : VV019017.D
Acq On : 20 Oct 2020 16:22
Operator : SY/MD
Sample : L4430-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc