

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019030.D
 Acq On : 20 Oct 2020 23:30
 Operator : SY/MD
 Sample : VIBLK75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	113168	113176	9.67%	1.254%
2	1.579	145	152	166	rVB	125228	140950	12.04%	1.561%
3	2.122	312	321	351	rVB	234596	372995	31.86%	4.131%
4	3.145	634	639	641	rBV3	675	692	0.06%	0.008%
5	3.482	740	744	750	rBV4	481	446	0.04%	0.005%
6	3.785	836	838	842	rBV2	357	182	0.02%	0.002%
7	3.917	868	879	916	rBV	90206	297221	25.38%	3.292%
8	4.376	1007	1022	1048	rBV	192436	469215	40.07%	5.197%
9	4.804	1153	1155	1160	rBV2	356	299	0.03%	0.003%
10	5.071	1222	1238	1279	rBV2	455376	1170890	100.00%	12.969%
11	5.489	1365	1368	1370	rBV2	405	239	0.02%	0.003%
12	5.640	1403	1415	1443	rBV	400576	806845	68.91%	8.937%
13	5.929	1493	1505	1526	rBV2	44390	93654	8.00%	1.037%
14	6.093	1542	1556	1581	rBV	275935	556043	47.49%	6.159%
15	6.373	1641	1643	1645	rBV	453	203	0.02%	0.002%
16	6.421	1655	1658	1662	rBV2	446	435	0.04%	0.005%
17	6.585	1708	1709	1713	rVB2	330	172	0.01%	0.002%
18	6.646	1723	1728	1730	rBV2	841	831	0.07%	0.009%
19	6.752	1757	1761	1766	rBV3	635	552	0.05%	0.006%
20	6.833	1784	1786	1787	rVB	272	58	0.00%	0.001%
21	7.010	1829	1841	1860	rBV	132552	244821	20.91%	2.712%
22	7.338	1931	1943	1971	rBV	501963	867247	74.07%	9.606%
23	7.643	2028	2038	2065	rBV	97794	173114	14.78%	1.917%
24	7.965	2134	2138	2140	rBV2	596	455	0.04%	0.005%
25	8.000	2141	2149	2159	rVB4	9025	16325	1.39%	0.181%
26	8.109	2173	2183	2222	rBV2	289124	604588	51.63%	6.697%
27	8.633	2343	2346	2348	rBV2	655	388	0.03%	0.004%
28	8.871	2409	2420	2447	rBV	627986	1008758	86.15%	11.173%
29	9.228	2530	2531	2534	rBV2	235	121	0.01%	0.001%
30	9.357	2566	2571	2574	rBV2	367	344	0.03%	0.004%
31	9.482	2608	2610	2611	rBV2	245	81	0.01%	0.001%
32	9.691	2671	2675	2678	rBV	343	238	0.02%	0.003%
33	9.710	2678	2681	2682	rBV	221	120	0.01%	0.001%
34	9.932	2747	2750	2756	rBV	256	259	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019030.D
 Acq On : 20 Oct 2020 23:30
 Operator : SY/MD
 Sample : VIBLK75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	10.026	2774	2779	2781	rBV2	437	302	0.03%	0.003%
36	10.048	2784	2786	2791	rVB2	566	338	0.03%	0.004%
37	10.074	2791	2794	2795	rBV	247	110	0.01%	0.001%
38	10.106	2801	2804	2806	rBV	148	102	0.01%	0.001%
39	10.138	2811	2814	2819	rVB	233	187	0.02%	0.002%
40	10.164	2819	2822	2827	rBV2	273	298	0.03%	0.003%
41	10.196	2828	2832	2833	rVV2	375	274	0.02%	0.003%
42	10.235	2833	2844	2869	rVB	274382	432919	36.97%	4.795%
43	10.321	2869	2871	2873	rBV3	371	173	0.01%	0.002%
44	10.347	2876	2879	2882	rBV3	402	320	0.03%	0.004%
45	10.379	2887	2889	2892	rVB	399	209	0.02%	0.002%
46	10.402	2893	2896	2897	rBV	203	94	0.01%	0.001%
47	10.418	2899	2901	2906	rVB2	336	222	0.02%	0.002%
48	10.444	2906	2909	2914	rVB2	361	294	0.03%	0.003%
49	10.473	2914	2918	2919	rBV2	319	209	0.02%	0.002%
50	10.579	2948	2951	2954	rBV	229	190	0.02%	0.002%
51	10.601	2954	2958	2959	rBV2	239	165	0.01%	0.002%
52	10.682	2982	2983	2984	rBV2	112	23	0.00%	0.000%
53	10.781	3011	3014	3019	rVB2	363	304	0.03%	0.003%
54	10.936	3061	3062	3064	rVB	126	47	0.00%	0.001%
55	10.948	3064	3066	3068	rBV2	151	83	0.01%	0.001%
56	11.006	3082	3084	3088	rBV	372	218	0.02%	0.002%
57	11.083	3105	3108	3111	rBV	221	154	0.01%	0.002%
58	11.141	3124	3126	3128	rBV2	126	60	0.01%	0.001%
59	11.186	3138	3140	3142	rBV	318	104	0.01%	0.001%
60	11.206	3142	3146	3153	rVB4	355	430	0.04%	0.005%
61	11.270	3153	3166	3192	rBV	547286	848102	72.43%	9.394%
62	11.408	3207	3209	3212	rVB2	597	274	0.02%	0.003%
63	11.489	3232	3234	3237	rVB2	265	119	0.01%	0.001%
64	11.508	3237	3240	3243	rBV	413	314	0.03%	0.003%
65	11.553	3252	3254	3259	rVB2	318	167	0.01%	0.002%
66	11.582	3259	3263	3266	rBV2	260	160	0.01%	0.002%
67	11.646	3270	3283	3302	rBV	504947	794787	67.88%	8.803%
68	11.919	3365	3368	3372	rBV2	386	317	0.03%	0.004%
69	12.167	3439	3445	3448	rBV2	357	360	0.03%	0.004%
70	12.235	3463	3466	3469	rBV	386	360	0.03%	0.004%
71	12.353	3500	3503	3504	rBV	273	152	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
Data File : VV019030.D
Acq On : 20 Oct 2020 23:30
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis

72	12.469	3536	3539	3540	rBV	173	89	0.01%	0.001%
73	12.534	3556	3559	3560	rBV	290	134	0.01%	0.001%
74	12.556	3563	3566	3572	rVB	542	474	0.04%	0.005%
75	12.588	3572	3576	3578	rBV	394	234	0.02%	0.003%
76	12.784	3633	3637	3640	rVB	264	242	0.02%	0.003%
77	12.855	3657	3659	3662	rBV	206	104	0.01%	0.001%
78	12.871	3662	3664	3666	rBV	258	152	0.01%	0.002%
79	13.093	3728	3733	3737	rBV3	480	624	0.05%	0.007%
80	13.296	3794	3796	3804	rBV3	409	407	0.03%	0.005%
81	13.945	3996	3998	4000	rBV2	203	120	0.01%	0.001%
82	14.096	4042	4045	4048	rBV3	505	351	0.03%	0.004%
83	14.115	4048	4051	4053	rVV2	347	182	0.02%	0.002%
84	14.373	4128	4131	4132	rBV	399	208	0.02%	0.002%


Sum of corrected areas: 9028219

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102020\
Data File : VV019030.D
Acq On : 20 Oct 2020 23:30
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

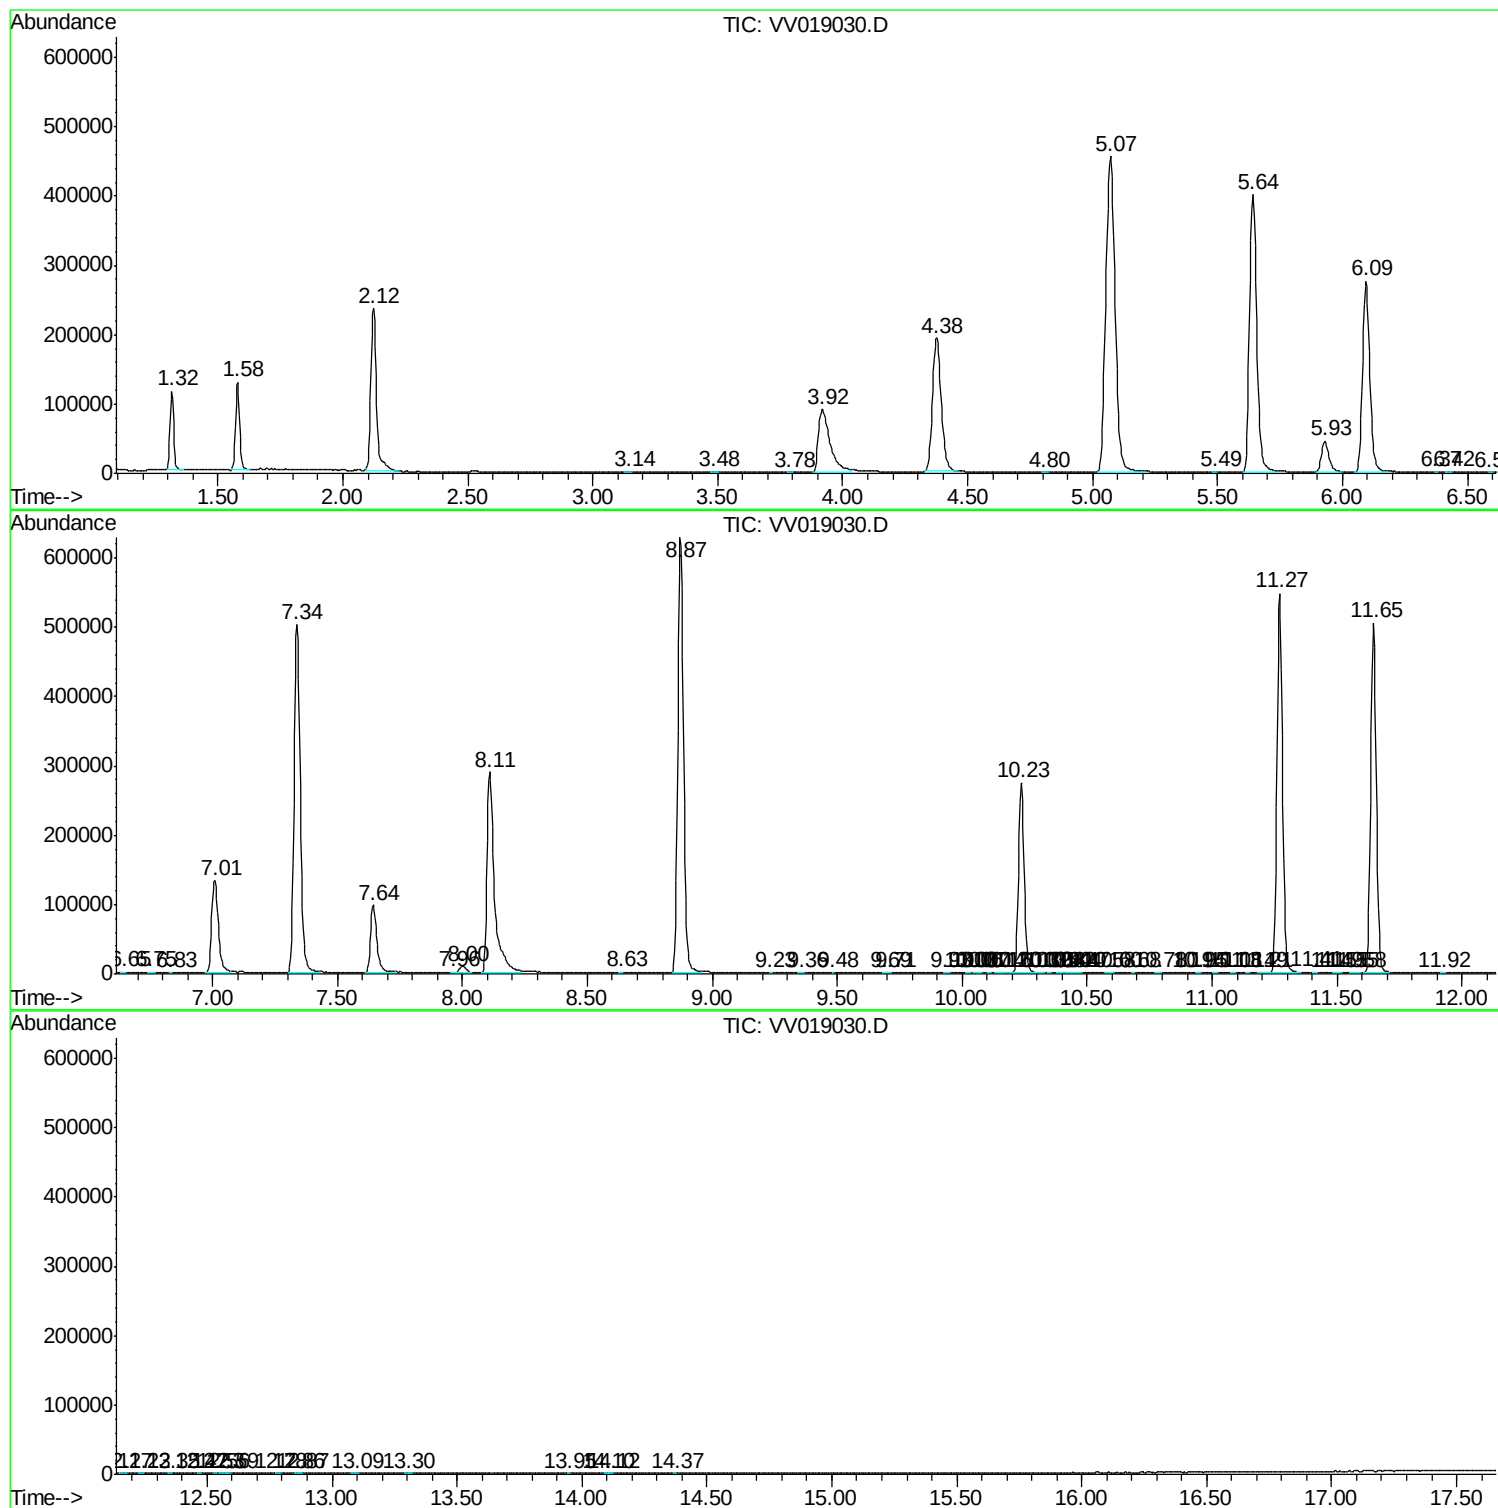

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102020\
Data File : VV019030.D
Acq On : 20 Oct 2020 23:30
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102020\
Data File : VV019030.D
Acq On : 20 Oct 2020 23:30
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc