

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019031.D
 Acq On : 20 Oct 2020 23:53
 Operator : SY/MD
 Sample : L4430-09 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.318	63	71	90	rVB2	577949	609544	13.28%	3.177%
2	1.579	145	152	163	rBV	121628	138439	3.02%	0.722%
3	2.116	310	319	349	rVB2	247978	401955	8.76%	2.095%
4	2.630	469	479	491	rVB4	2655	5986	0.13%	0.031%
5	2.679	493	494	498	rBV2	212	148	0.00%	0.001%
6	2.730	507	510	512	rBV2	419	298	0.01%	0.002%
7	2.778	514	525	540	rVV	33353	60568	1.32%	0.316%
8	2.942	574	576	578	rBV	149	82	0.00%	0.000%
9	2.968	582	584	585	rBV	248	86	0.00%	0.000%
10	3.087	619	621	623	rBV	360	183	0.00%	0.001%
11	3.129	632	634	636	rVB	155	59	0.00%	0.000%
12	3.196	651	655	657	rBV2	340	244	0.01%	0.001%
13	3.235	662	667	669	rBV2	506	447	0.01%	0.002%
14	3.354	702	704	705	rBV	290	131	0.00%	0.001%
15	3.363	705	707	709	rVV	226	121	0.00%	0.001%
16	3.441	726	731	732	rBV2	337	241	0.01%	0.001%
17	3.498	745	749	755	rBV4	393	562	0.01%	0.003%
18	3.563	764	769	772	rVB2	275	223	0.00%	0.001%
19	3.585	772	776	778	rBV	342	243	0.01%	0.001%
20	3.672	797	803	807	rVB3	341	354	0.01%	0.002%
21	3.736	817	823	827	rVB2	319	332	0.01%	0.002%
22	3.765	829	832	836	rBV	334	205	0.00%	0.001%
23	3.794	839	841	842	rBV	251	113	0.00%	0.001%
24	3.846	854	857	858	rBV	325	140	0.00%	0.001%
25	3.933	867	884	914	rBV2	1421069	3522606	76.77%	18.360%
26	4.373	1006	1021	1049	rBV	167375	418191	9.11%	2.180%
27	4.630	1098	1101	1104	rBV	219	159	0.00%	0.001%
28	4.695	1119	1121	1126	rBV2	484	487	0.01%	0.003%
29	4.794	1150	1152	1155	rBV3	253	174	0.00%	0.001%
30	4.855	1168	1171	1173	rVB2	346	151	0.00%	0.001%
31	4.904	1182	1186	1189	rBV2	372	364	0.01%	0.002%
32	4.984	1208	1211	1215	rVB2	349	286	0.01%	0.001%
33	5.003	1215	1217	1220	rBV2	176	119	0.00%	0.001%
34	5.071	1220	1238	1263	rBV2	396874	1022534	22.28%	5.329%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
 Data File : VV019031.D
 Acq On : 20 Oct 2020 23:53
 Operator : SY/MD
 Sample : L4430-09 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	5.482	1363	1366	1369	rBV2	387	224	0.00%	0.001%
36	5.498	1369	1371	1373	rBV	266	163	0.00%	0.001%
37	5.537	1381	1383	1385	rBV2	353	179	0.00%	0.001%
38	5.582	1395	1397	1400	rVB	240	146	0.00%	0.001%
39	5.640	1402	1415	1448	rBV	357601	715848	15.60%	3.731%
40	5.936	1492	1507	1542	rBV	1209502	2347538	51.16%	12.235%
41	6.093	1544	1556	1583	rVB	237279	484899	10.57%	2.527%
42	6.283	1612	1615	1617	rBV2	393	271	0.01%	0.001%
43	6.376	1641	1644	1645	rBV	290	178	0.00%	0.001%
44	6.653	1725	1730	1732	rBV4	839	768	0.02%	0.004%
45	6.781	1766	1770	1774	rVB2	421	378	0.01%	0.002%
46	6.817	1774	1781	1782	rBV2	386	437	0.01%	0.002%
47	6.894	1802	1805	1812	rVB2	505	542	0.01%	0.003%
48	6.926	1813	1815	1817	rBV2	208	117	0.00%	0.001%
49	7.006	1829	1840	1864	rBV	120626	221716	4.83%	1.156%
50	7.338	1931	1943	1968	rBV	446483	778149	16.96%	4.056%
51	7.643	2027	2038	2057	rBV	90704	159754	3.48%	0.833%
52	7.874	2102	2110	2114	rBV3	1184	1759	0.04%	0.009%
53	7.916	2120	2123	2125	rBV2	199	153	0.00%	0.001%
54	7.997	2134	2148	2174	rBV	2782296	4588775	100.00%	23.916%
55	8.112	2175	2184	2221	rVB2	232708	555346	12.10%	2.894%
56	8.376	2262	2266	2270	rBV3	650	625	0.01%	0.003%
57	8.588	2330	2332	2334	rBV3	431	229	0.00%	0.001%
58	8.643	2346	2349	2355	rBV2	470	472	0.01%	0.002%
59	8.871	2409	2420	2442	rBV	557861	906396	19.75%	4.724%
60	9.170	2509	2513	2514	rBV2	418	284	0.01%	0.001%
61	9.231	2527	2532	2537	rVB2	427	495	0.01%	0.003%
62	9.264	2537	2542	2545	rBV2	374	449	0.01%	0.002%
63	9.337	2562	2565	2568	rVB2	488	262	0.01%	0.001%
64	9.415	2586	2589	2591	rBV2	414	298	0.01%	0.002%
65	9.489	2609	2612	2614	rBV2	131	81	0.00%	0.000%
66	9.505	2614	2617	2621	rBV2	379	304	0.01%	0.002%
67	9.563	2633	2635	2639	rBV2	517	436	0.01%	0.002%
68	9.781	2699	2703	2706	rBV3	457	414	0.01%	0.002%
69	10.196	2828	2832	2834	rBV3	345	248	0.01%	0.001%
70	10.238	2834	2845	2862	rVV	285678	461846	10.06%	2.407%
71	10.353	2878	2881	2885	rBV3	296	210	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102020\
Data File : VV019031.D
Acq On : 20 Oct 2020 23:53
Operator : SY/MD
Sample : L4430-09 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis

72	10.501	2925	2927	2929	rBV2	239	147	0.00%	0.001%
73	10.537	2935	2938	2940	rBV	167	105	0.00%	0.001%
74	10.720	2992	2995	3000	rBV2	400	465	0.01%	0.002%
75	11.215	3145	3149	3155	rVB4	1038	1017	0.02%	0.005%
76	11.270	3155	3166	3189	rBV	609086	932214	20.32%	4.859%
77	11.646	3270	3283	3302	rBV	537274	836195	18.22%	4.358%
78	12.366	3503	3507	3509	rBV2	317	254	0.01%	0.001%
79	13.617	3894	3896	3900	rBV2	281	179	0.00%	0.001%


Sum of corrected areas: 19186740

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102020\
Data File : VV019031.D
Acq On : 20 Oct 2020 23:53
Operator : SY/MD
Sample : L4430-09 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

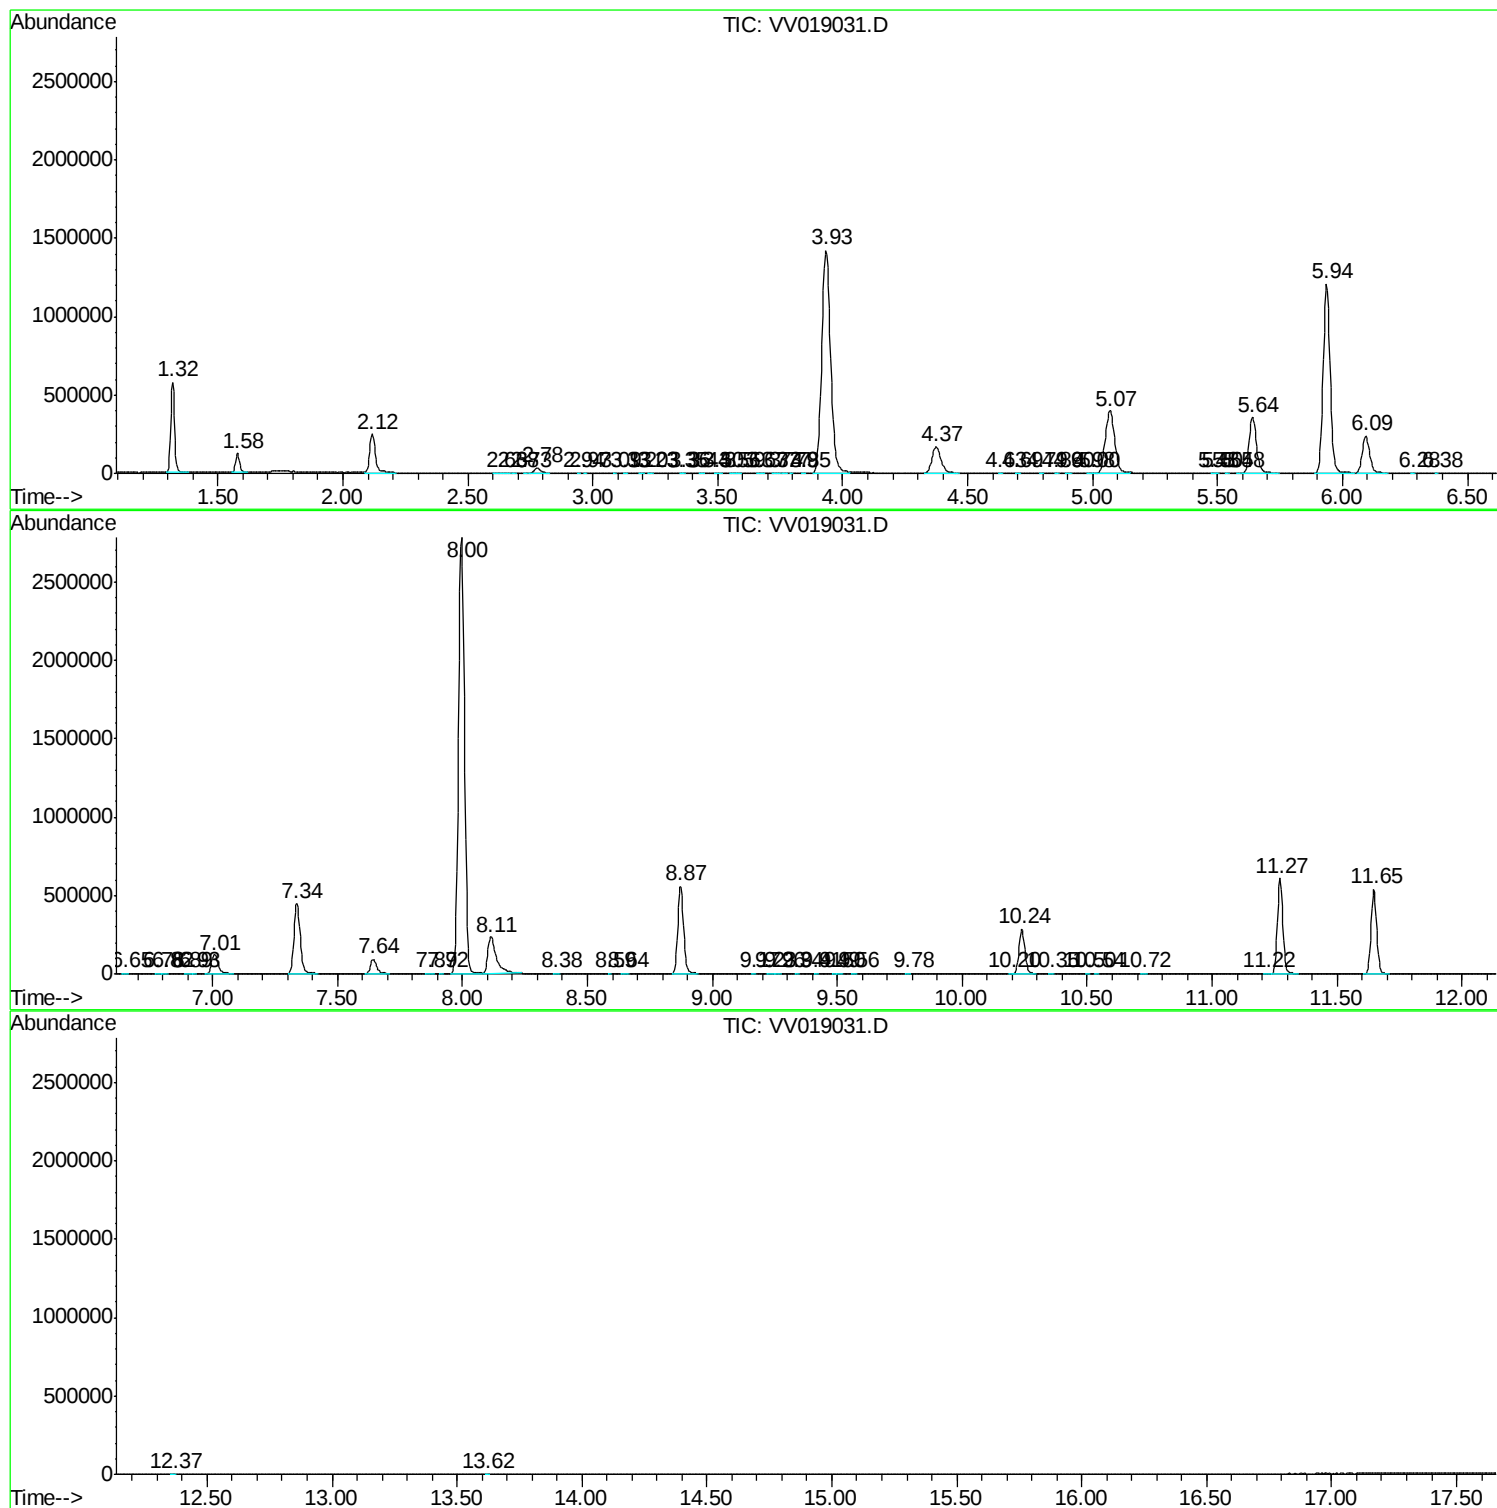

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102020\
Data File : VV019031.D
Acq On : 20 Oct 2020 23:53
Operator : SY/MD
Sample : L4430-09 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102020\
Data File : VV019031.D
Acq On : 20 Oct 2020 23:53
Operator : SY/MD
Sample : L4430-09 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc