


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102020\
Data File : VV019000.D
Acq On : 20 Oct 2020 08:48
Operator : SY/MD
Sample : BFB78
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB78

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis
Last Update : Wed Oct 21 11:19:02 2020

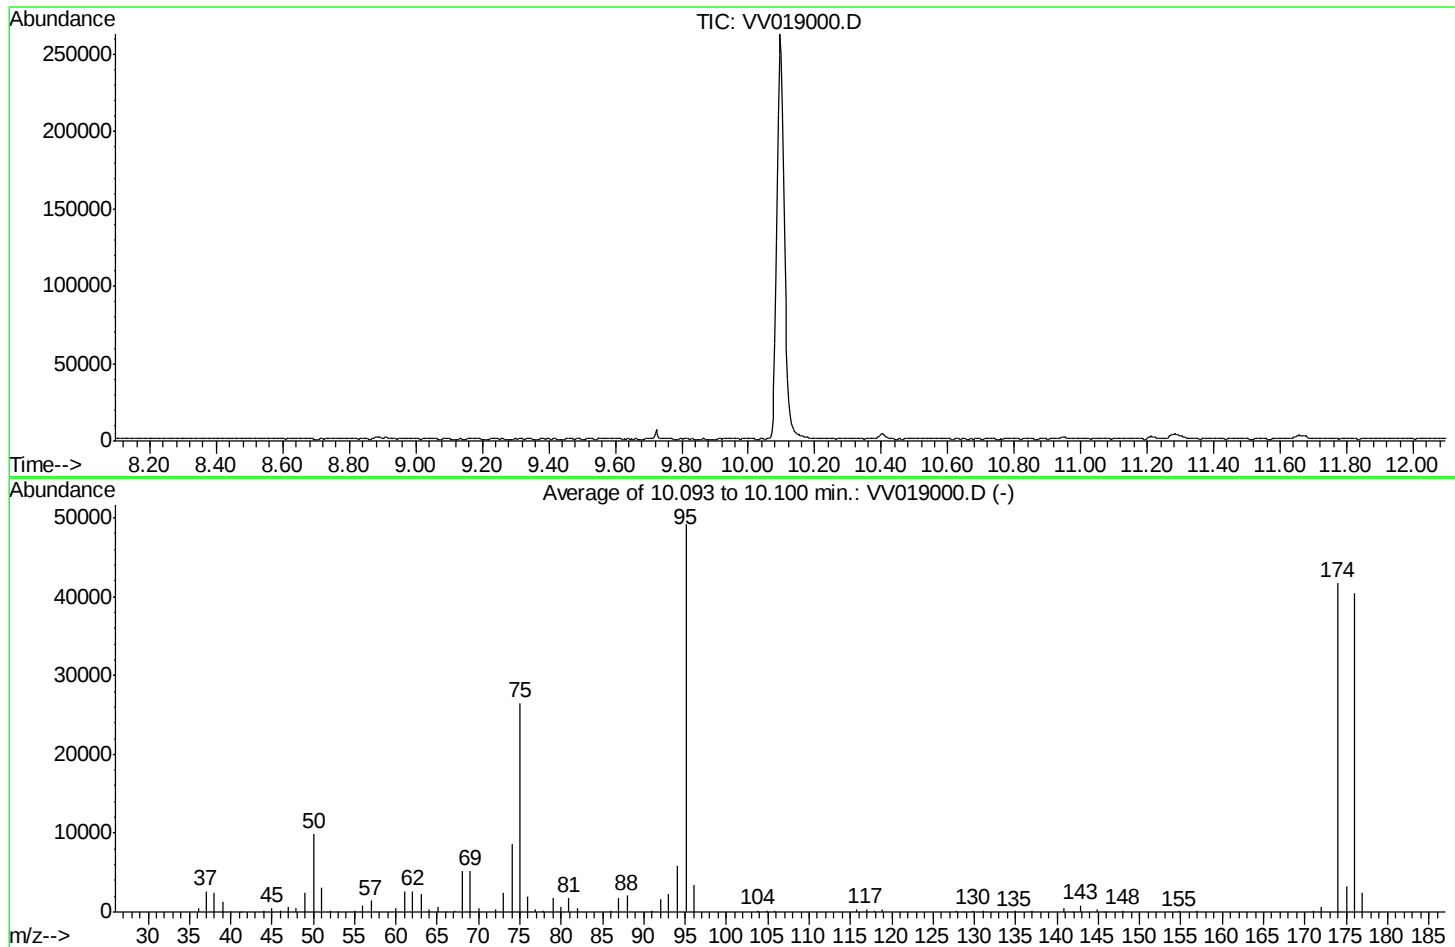

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	9944	PASS
75	95	30	80	53.9	26520	PASS
95	95	100	100	100.0	49168	PASS
96	95	5	9	6.9	3382	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.9	41768	PASS
175	174	5	9	7.9	3286	PASS
176	174	95	101	96.7	40378	PASS
177	176	5	9	6.2	2486	PASS

m/z	Abundance
36.10	578.0
37.00	2728.0
38.00	2506.0
39.00	1205.0
40.00	314.0
44.00	1302.0
45.00	524.0
46.00	200.0
47.00	765.0
47.90	390.0
49.00	2439.0
50.10	10057.0
51.00	3272.0
52.00	181.0
53.00	141.0
55.10	159.0
56.00	826.0
57.00	1315.0
60.00	586.0
61.00	2633.0
62.00	2713.0
63.00	2150.0
64.00	345.0
65.10	659.0
66.00	117.0
67.10	171.0
68.00	5048.0
69.00	5362.0
70.00	574.0
72.00	284.0
73.00	2369.0
74.00	8787.0
75.00	26192.0
76.00	2014.0
76.90	348.0
77.90	208.0
79.00	1790.0
79.90	566.0
80.90	1824.0
81.90	450.0
86.00	140.0
87.00	1895.0
88.00	1924.0
90.90	212.0
92.00	1569.0
93.00	2286.0
94.10	5836.0
95.10	48272.0
96.00	3425.0
103.80	209.0
104.90	116.0
105.90	199.0
115.80	209.0
116.90	361.0
117.90	178.0
118.90	324.0
127.80	189.0
129.90	235.0
131.10	100.0
134.90	136.0
136.90	104.0
140.90	524.0
142.90	748.0
144.90	350.0
145.70	110.0
148.00	180.0
154.90	121.0
156.80	111.0
171.00	146.0
172.00	699.0
174.00	40072.0
175.00	3035.0
176.00	39008.0
177.00	2384.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.10	553.0
37.00	2778.0
38.10	2522.0
39.00	1347.0
40.00	293.0
44.10	1298.0
45.00	573.0
46.00	172.0
47.00	778.0
47.90	457.0
49.00	2479.0
50.10	10214.0
51.00	3227.0
52.00	179.0
52.90	121.0
54.90	175.0
56.00	820.0
57.00	1426.0
60.00	583.0
61.00	2664.0
62.00	2737.0
63.00	2354.0
64.00	359.0
65.10	728.0
66.00	116.0
67.10	160.0
68.00	5375.0
69.00	5521.0
70.00	568.0
72.00	340.0
73.00	2459.0
74.00	8879.0
75.10	27536.0
76.00	2032.0
76.90	330.0
77.90	254.0
79.00	1869.0
79.90	595.0
81.00	1913.0
81.90	466.0
86.00	160.0
87.00	1909.0
88.00	2194.0
90.90	227.0
92.00	1742.0
93.00	2281.0
94.10	6086.0
95.10	51040.0
96.00	3515.0
103.80	221.0
104.90	140.0
105.90	192.0
115.80	263.0
116.90	350.0
117.80	190.0
118.90	333.0
127.90	175.0
129.90	268.0
131.00	112.0
134.90	149.0
136.90	124.0
140.90	594.0
141.90	120.0
142.90	860.0
144.90	328.0
145.70	126.0
148.00	197.0
154.80	160.0
156.90	119.0
171.00	164.0
172.00	700.0
174.00	43064.0
175.00	3424.0
176.00	41816.0
177.00	2571.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.00	483.0
37.00	2484.0
38.00	2328.0
39.00	1248.0
40.00	298.0
41.20	114.0
44.00	1325.0
45.00	521.0
45.90	111.0
47.00	657.0
47.90	452.0
49.00	2257.0
50.10	9562.0
51.00	2871.0
52.00	134.0
55.10	182.0
56.00	750.0
57.00	1427.0
60.00	520.0
61.00	2464.0
62.00	2447.0
63.00	2280.0
64.00	326.0
65.10	708.0
67.10	129.0
68.00	5111.0
69.00	4919.0
70.00	546.0
72.00	367.0
73.00	2337.0
74.00	8187.0
75.10	25832.0
76.00	1911.0
76.90	273.0
77.80	248.0
78.90	1771.0
79.90	594.0
81.00	1819.0
81.90	438.0
87.00	1805.0
88.00	2140.0
91.00	227.0
92.00	1577.0
93.00	2131.0
94.10	5795.0
95.10	48192.0
96.10	3207.0
103.90	237.0
104.90	127.0
105.90	202.0
115.80	314.0
116.90	340.0
117.80	180.0
118.90	338.0
127.90	187.0
128.70	116.0
129.90	244.0
131.00	123.0
134.90	132.0
136.90	134.0
140.90	591.0
141.90	118.0
142.90	840.0
144.90	259.0
145.90	151.0
148.00	174.0
154.80	171.0
157.00	138.0
171.00	140.0
172.00	682.0
174.00	42168.0
175.00	3399.0
176.00	40312.0
177.00	2505.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

Scan 2790 (10.061 min): VV019000.D
BFB78

m/z	Abundance
40.00	287.0
44.00	1163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78