


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022932.D
Acq On : 20 Oct 2021 15:18
Operator : SY/MD
Sample : M4200-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE8

Manual Integrations
APPROVED

MMDadoda
10/22/2021 11:29:05 AM

Quant Time: Oct 21 02:46:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 21 02:43:59 2021
Response via : Initial Calibration

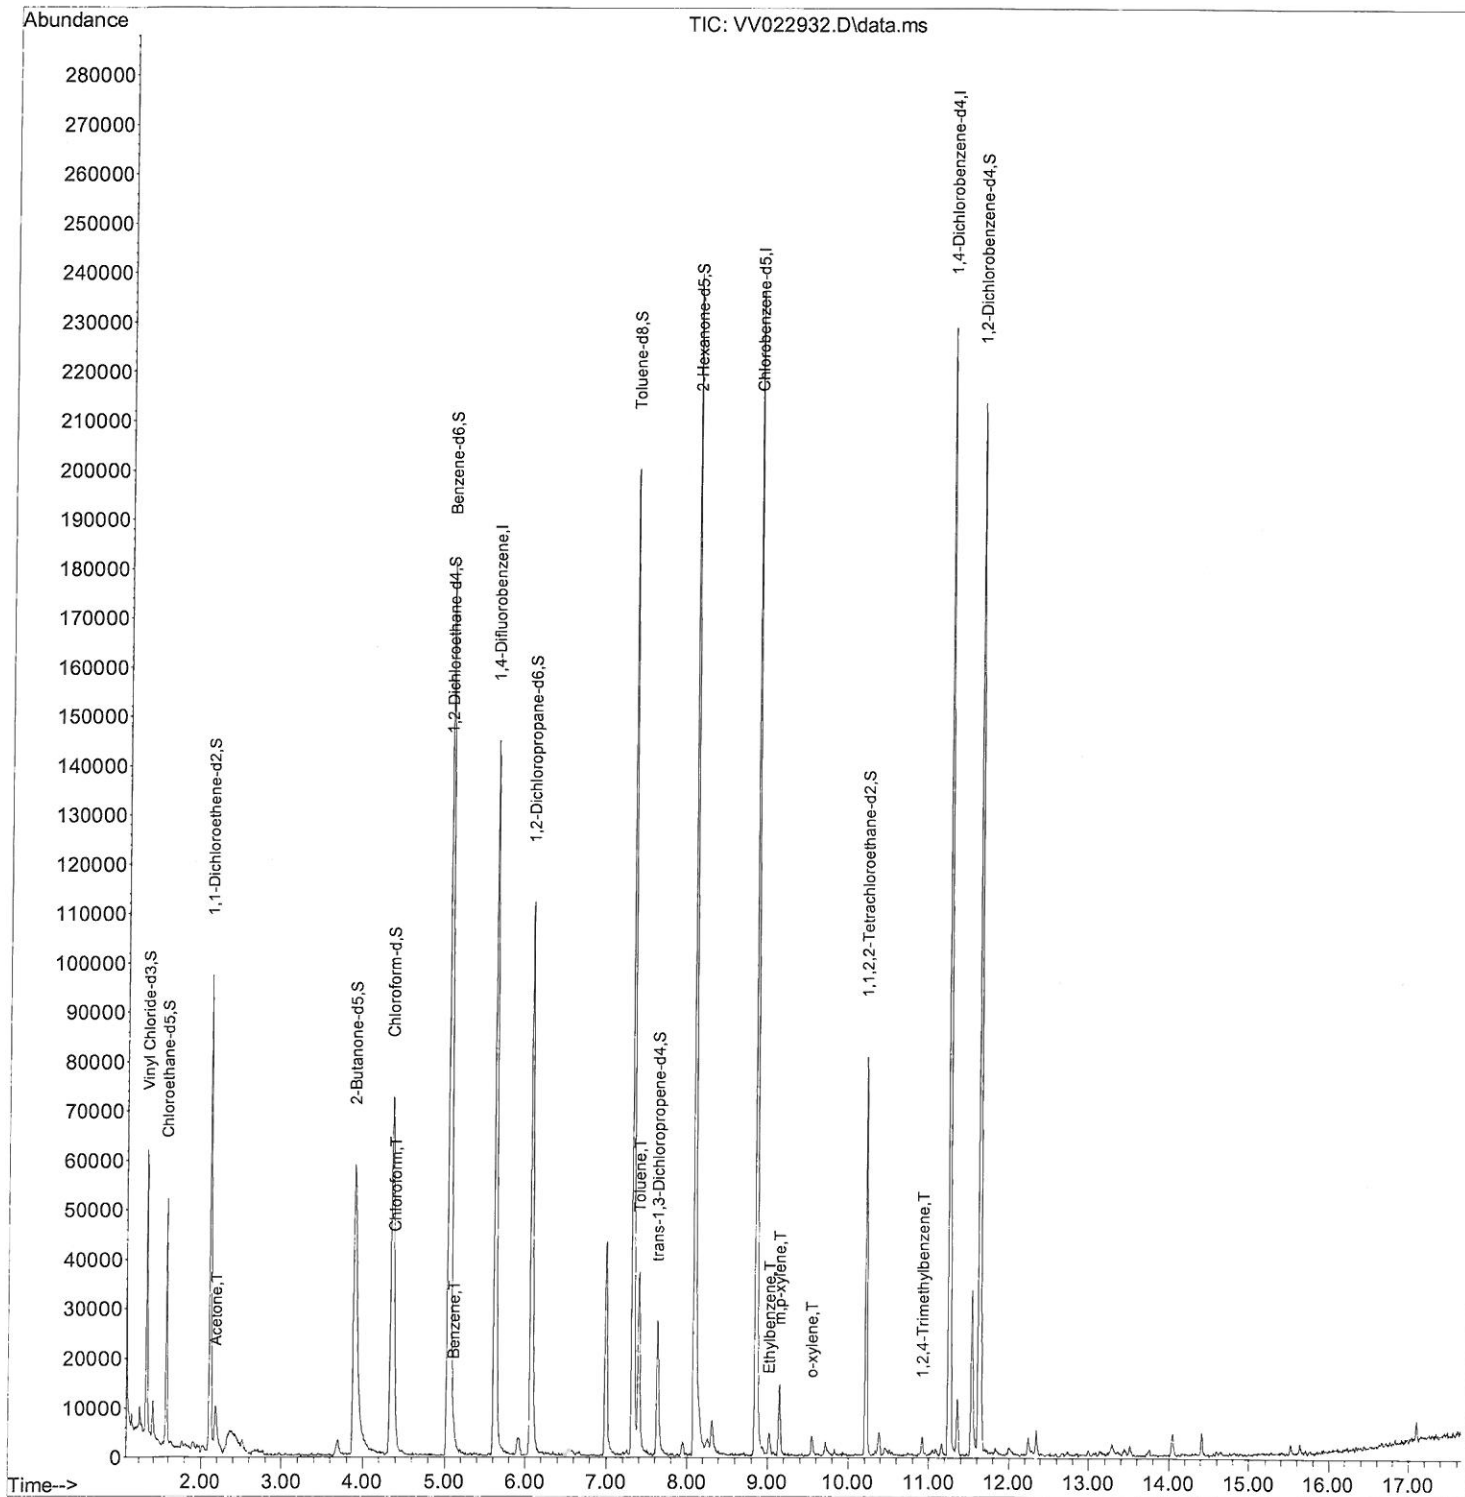




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022932.D
Acq On : 20 Oct 2021 15:18
Operator : SY/MD
Sample : M4200-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGES

Manual Integrations
APPROVED

MMDadoda
10/22/2021 11:29:05 AM

Quant Time: Oct 21 02:46:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 21 02:43:59 2021
Response via : Initial Calibration

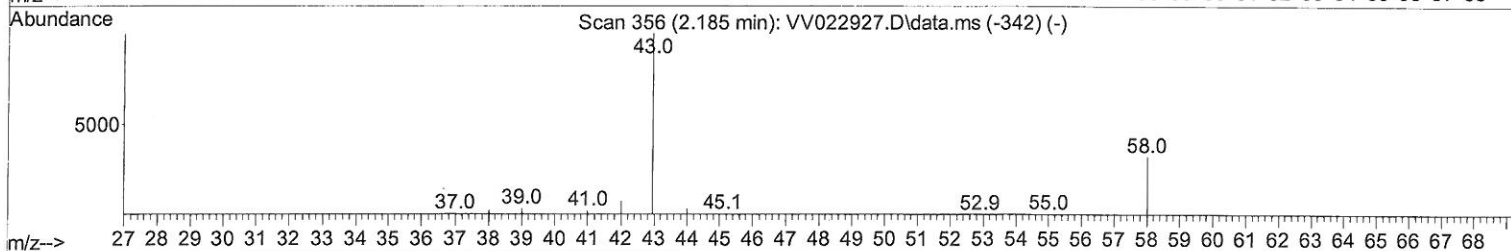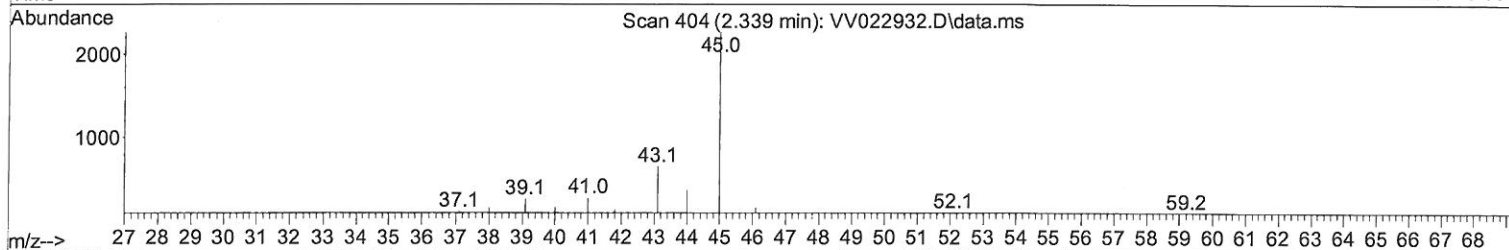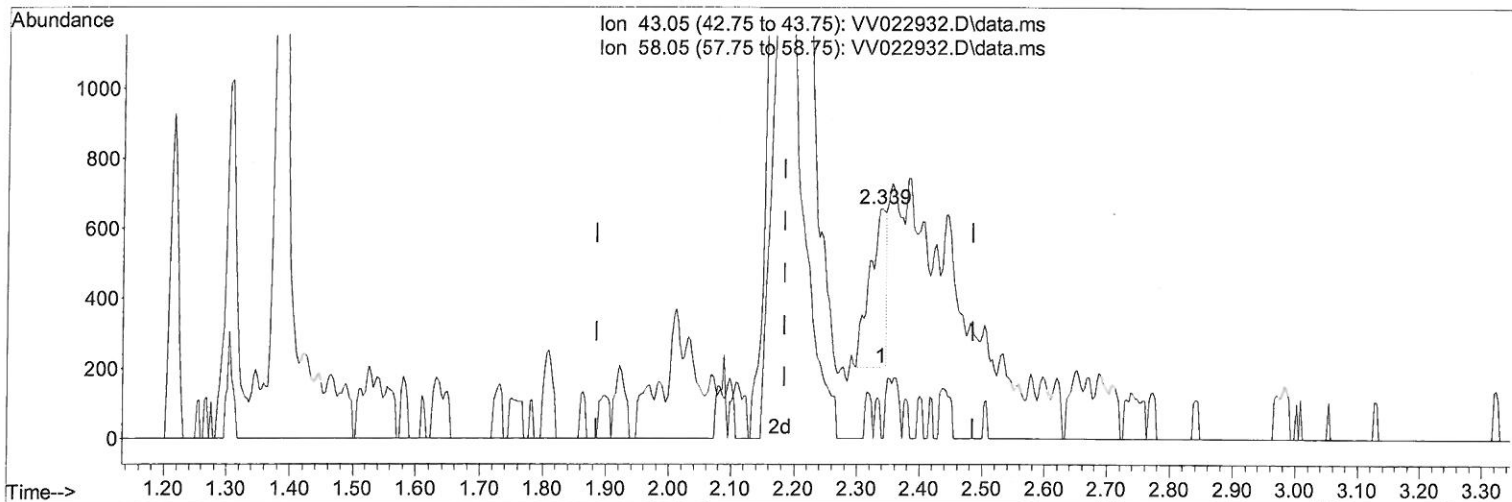

TIC: VV022932.D\data.ms

(13) Acetone (T)

2.339min (+ 0.154) 0.64 ug/L

response 823

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	20.90
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
 Data File : VV022932.D
 Acq On : 20 Oct 2021 15:18
 Operator : SY/MD
 Sample : M4200-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGES

Manual Integrations
 APPROVED

MMDadoda
 10/22/2021 11:29:05 AM

Quant Time: Oct 21 02:46:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 21 02:43:59 2021
 Response via : Initial Calibration

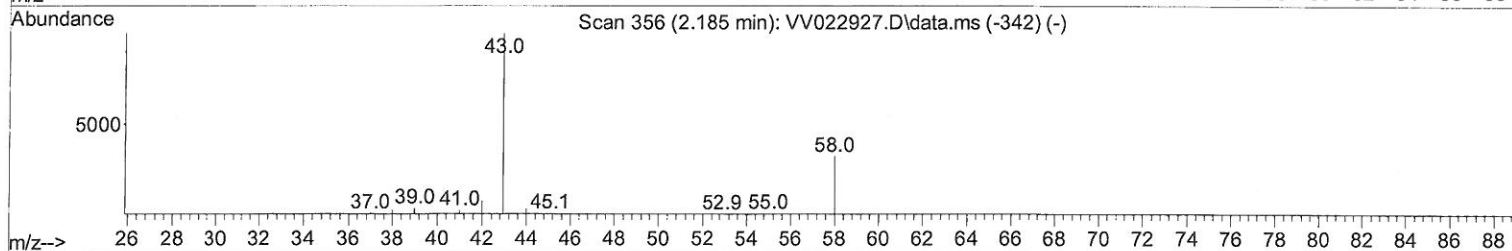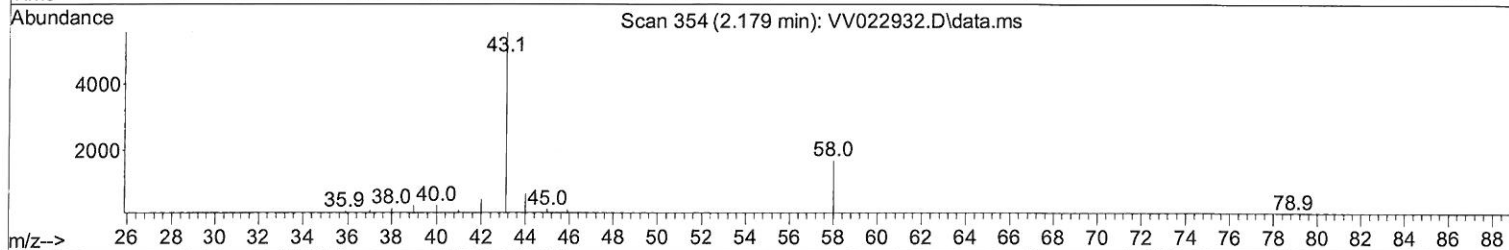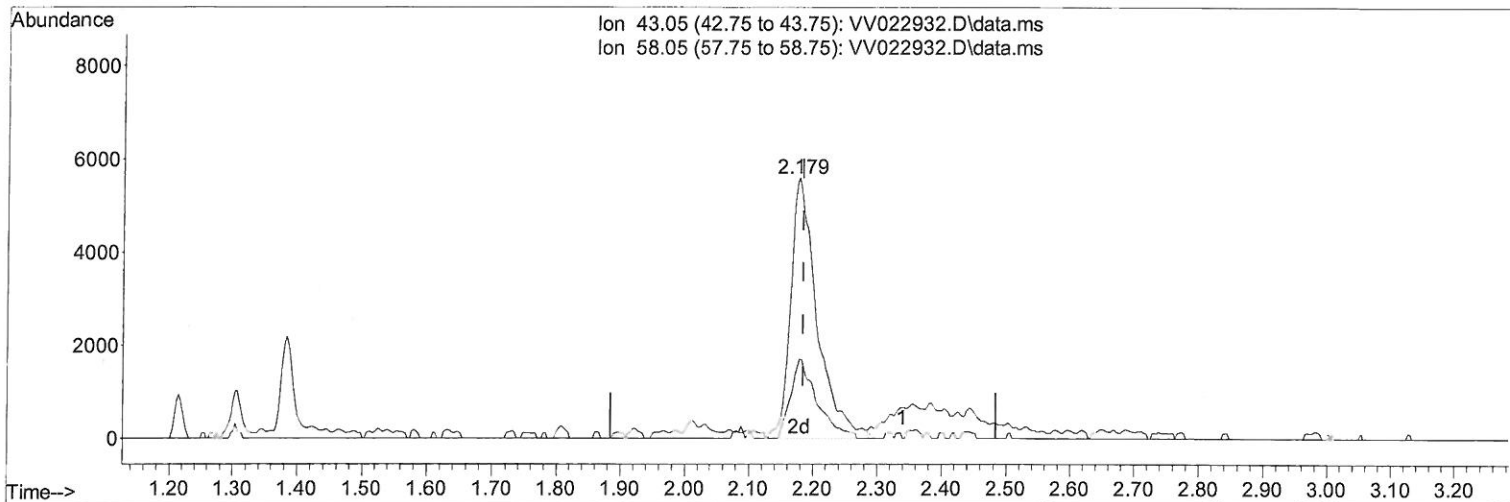

TIC: VV022932.D\data.ms

(13) Acetone (T)

2.179min (-0.006) 12.48 ug/L m

response 16040

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	1.07
0.00	0.00	0.00
0.00	0.00	0.00

> MD
 10/27/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
 Data File : VV022932.D
 Acq On : 20 Oct 2021 15:18
 Operator : SY/MD
 Sample : M4200-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG8

Manual Integrations
 APPROVED

MMDadoda
 10/22/2021 11:29:05 AM

Quant Time: Oct 21 02:46:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 21 02:43:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	127762	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	133893	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	63010	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	30840	3.508	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	70.200%	
7) Chloroethane-d5	1.568	69	30247	3.829	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	76.600%	
11) 1,1-Dichloroethene-d2	2.108	63	49303	2.859	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	57.200%#	
20) 2-Butanone-d5	3.889	46	105286	45.681	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	91.360%	
24) Chloroform-d	4.352	84	73209	4.041	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.800%	
26) 1,2-Dichloroethane-d4	5.037	65	41524	4.723	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.400%	
32) Benzene-d6	5.053	84	166358	4.174	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.400%	
36) 1,2-Dichloropropane-d6	6.072	67	55505	4.702	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	94.000%	
41) Toluene-d8	7.320	98	134385	3.900	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.000%	
43) trans-1,3-Dichloroprop...	7.625	79	16130	4.119	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.400%	
46) 2-Hexanone-d5	8.091	63	80124	50.775	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	101.540%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	37944	4.745	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	57158	4.893	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.800%	
Target Compounds						
13) Acetone	2.179	43	16040m	12.480	ug/L	Qvalue
25) Chloroform	4.381	83	16724	0.954	ug/L	93
33) Benzene	5.108	78	3537	0.098	ug/L	100
42) Toluene	7.394	91	27726	0.757	ug/L	97
52) Ethylbenzene	9.021	91	3244	0.087	ug/L	90
53) m,p-xylene	9.143	106	4292	0.294	ug/L	85
54) o-xylene	9.545	106	1258	0.092	ug/L #	58
63) 1,2,4-Trimethylbenzene	10.918	105	2302	0.089	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed