

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV102021\  
 Data File : VV022928.D  
 Acq On : 20 Oct 2021 12:44  
 Operator : SY/MD  
 Sample : VV1020WBL01  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VBLK228

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022928.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.304       | 75            | 82          | 97           | rVB      | 74072          | 76200         | 15.23%          | 1.919%        |
| 2         | 1.568       | 156           | 164         | 173          | rBV      | 52585          | 60166         | 12.02%          | 1.515%        |
| 3         | 2.108       | 318           | 332         | 351          | rBV      | 123572         | 177969        | 35.56%          | 4.483%        |
| 4         | 2.507       | 446           | 456         | 472          | rVB      | 16615          | 28186         | 5.63%           | 0.710%        |
| 5         | 3.899       | 878           | 889         | 916          | rBV2     | 33794          | 118774        | 23.73%          | 2.992%        |
| 6         | 4.349       | 1015          | 1029        | 1062         | rVB      | 84793          | 223478        | 44.66%          | 5.629%        |
| 7         | 5.050       | 1231          | 1247        | 1275         | rBV2     | 200002         | 500426        | 100.00%         | 12.604%       |
| 8         | 5.619       | 1412          | 1424        | 1442         | rBV      | 147367         | 301558        | 60.26%          | 7.595%        |
| 9         | 5.918       | 1506          | 1517        | 1521         | rBV6     | 3298           | 5769          | 1.15%           | 0.145%        |
| 10        | 6.072       | 1549          | 1565        | 1589         | rBV      | 115615         | 242891        | 48.54%          | 6.118%        |
| 11        | 6.992       | 1841          | 1851        | 1870         | rBV      | 48676          | 90238         | 18.03%          | 2.273%        |
| 12        | 7.317       | 1940          | 1952        | 1972         | rBV      | 229793         | 404861        | 80.90%          | 10.197%       |
| 13        | 7.625       | 2039          | 2048        | 2071         | rBV2     | 28644          | 54999         | 10.99%          | 1.385%        |
| 14        | 8.091       | 2182          | 2193        | 2236         | rBV      | 195302         | 438912        | 87.71%          | 11.055%       |
| 15        | 8.854       | 2419          | 2430        | 2455         | rBV      | 239222         | 397313        | 79.39%          | 10.007%       |
| 16        | 10.217      | 2843          | 2854        | 2871         | rBV      | 81246          | 133481        | 26.67%          | 3.362%        |
| 17        | 11.249      | 3164          | 3175        | 3196         | rBV      | 227807         | 359387        | 71.82%          | 9.052%        |
| 18        | 11.625      | 3281          | 3292        | 3312         | rBV      | 226795         | 355627        | 71.06%          | 8.957%        |




Sum of corrected areas: 3970235

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV102021\  
Data File : VV022928.D  
Acq On : 20 Oct 2021 12:44  
Operator : SY/MD  
Sample : VV1020WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK228

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR100721WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

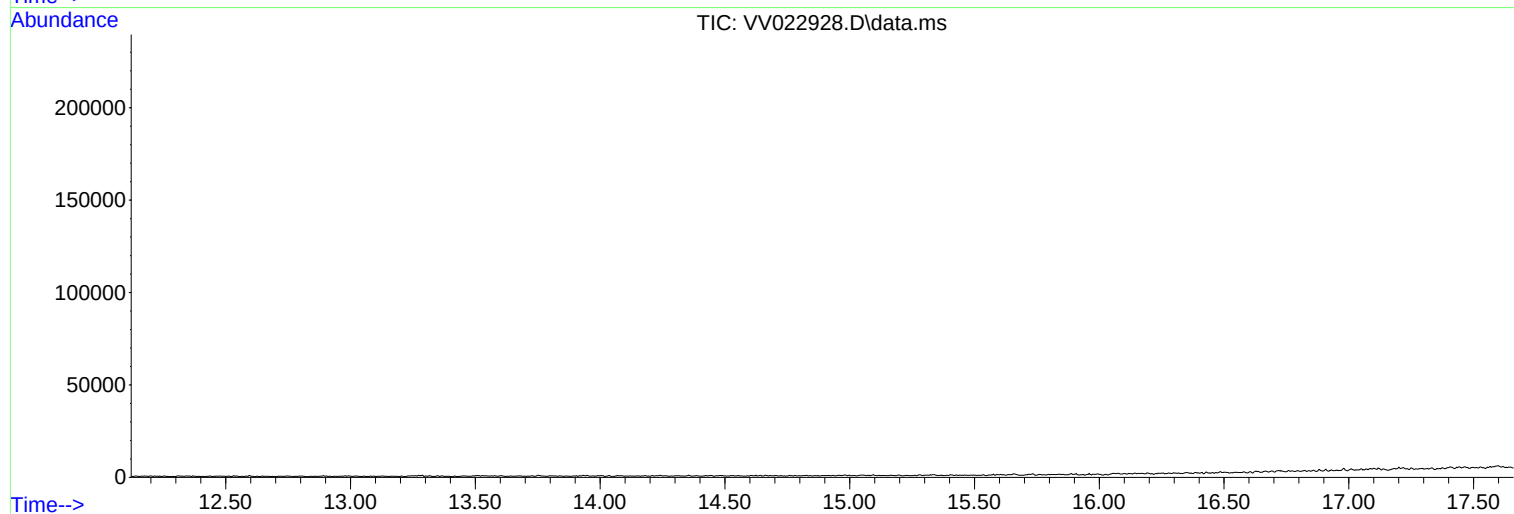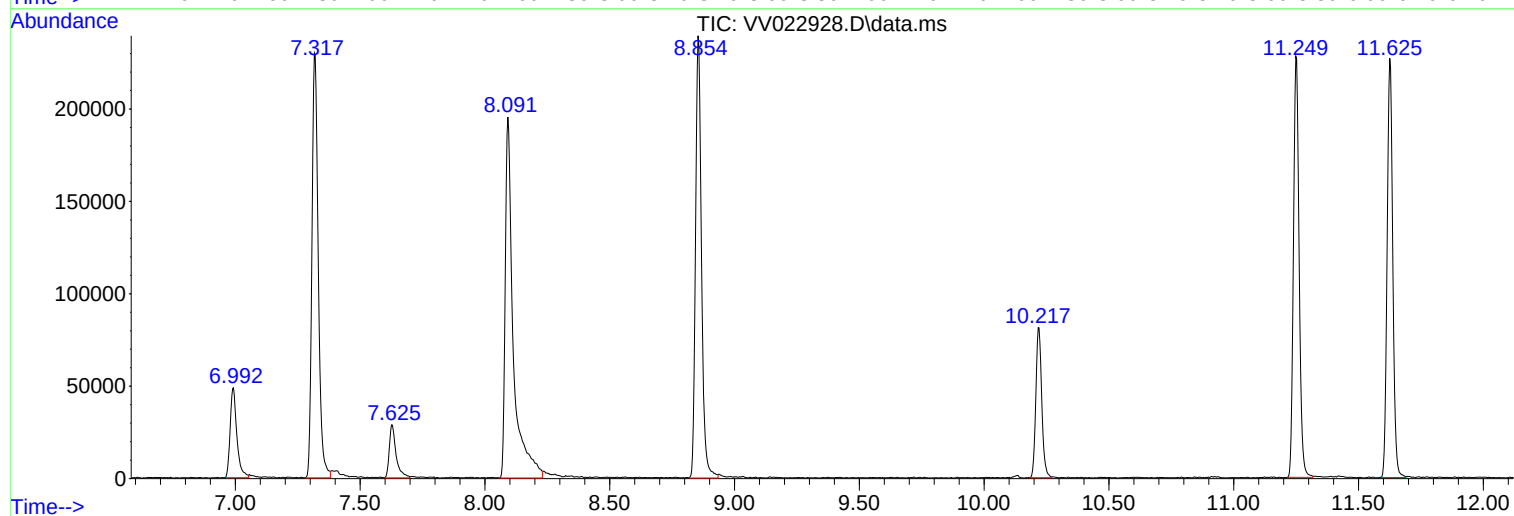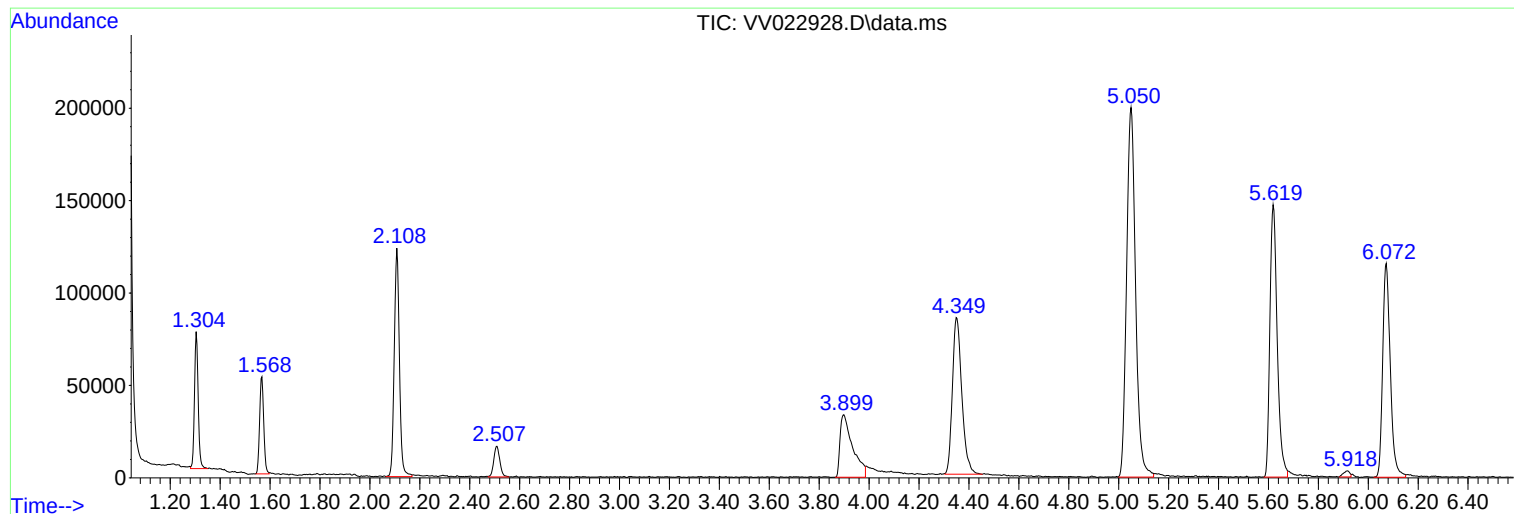

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV102021\  
Data File : VV022928.D  
Acq On : 20 Oct 2021 12:44  
Operator : SY/MD  
Sample : VV1020WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK228

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR100721WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV102021\  
Data File : VV022928.D  
Acq On : 20 Oct 2021 12:44  
Operator : SY/MD  
Sample : VV1020WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK228

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR100721WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----