

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
 Data File : VV022935.D
 Acq On : 20 Oct 2021 16:30
 Operator : SY/MD
 Sample : M4246-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022935.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	72363	76951	15.54%	1.971%
2	1.568	156	164	174	rVB	56352	62270	12.58%	1.595%
3	2.108	319	332	352	rBV	99154	144605	29.21%	3.704%
4	3.886	875	885	916	rBV2	51115	151165	30.53%	3.872%
5	4.352	1013	1030	1061	rBV3	78589	222325	44.90%	5.695%
6	5.050	1231	1247	1275	rBV2	195780	495116	100.00%	12.682%
7	5.619	1412	1424	1458	rBV	137134	284896	57.54%	7.297%
8	5.915	1506	1516	1532	rBV7	3166	6630	1.34%	0.170%
9	6.072	1552	1565	1598	rBV	118360	243583	49.20%	6.239%
10	6.989	1840	1850	1877	rBV	46132	91160	18.41%	2.335%
11	7.316	1941	1952	1971	rBV	226872	399013	80.59%	10.220%
12	7.400	1971	1978	1990	rVB4	5472	10993	2.22%	0.282%
13	7.625	2038	2048	2068	rBV2	28169	51229	10.35%	1.312%
14	7.940	2135	2146	2157	rVB3	9364	16368	3.31%	0.419%
15	8.091	2183	2193	2223	rBV	207769	378393	76.43%	9.692%
16	8.853	2419	2430	2453	rBV	219515	365086	73.74%	9.351%
17	10.217	2842	2854	2876	rBV2	77315	124287	25.10%	3.183%
18	10.384	2896	2906	2919	rVB2	21625	36356	7.34%	0.931%
19	11.249	3160	3175	3197	rBV	214406	337331	68.13%	8.640%
20	11.535	3253	3264	3274	rBV4	5464	9804	1.98%	0.251%
21	11.625	3280	3292	3316	rBV	225171	354736	71.65%	9.086%
22	12.255	3475	3488	3498	rBV2	11709	19864	4.01%	0.509%
23	14.043	4035	4044	4051	rBV2	4702	6801	1.37%	0.174%
24	17.097	4985	4994	5004	rBV	9396	15238	3.08%	0.390%




Sum of corrected areas: 3904200

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022935.D
Acq On : 20 Oct 2021 16:30
Operator : SY/MD
Sample : M4246-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

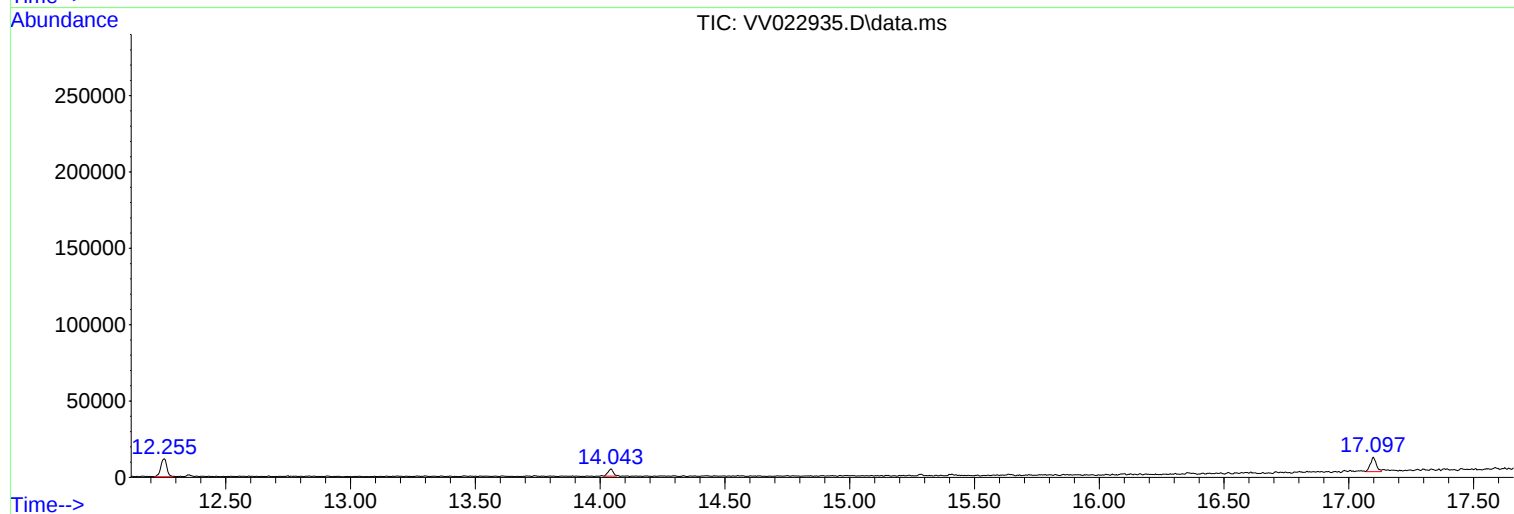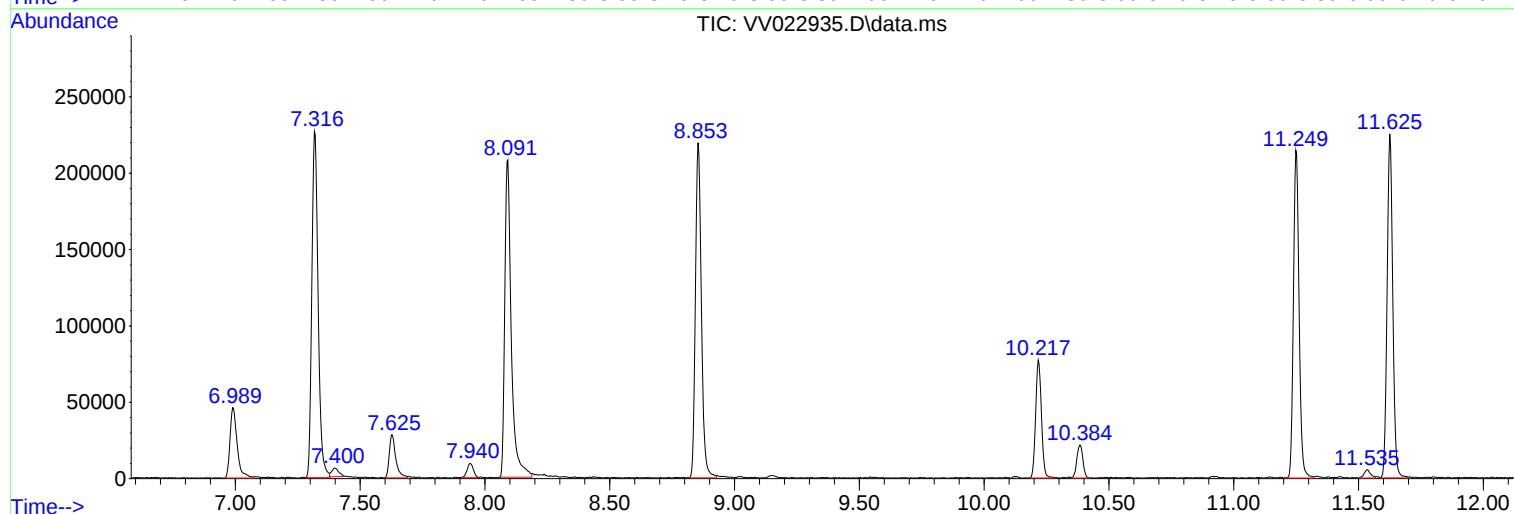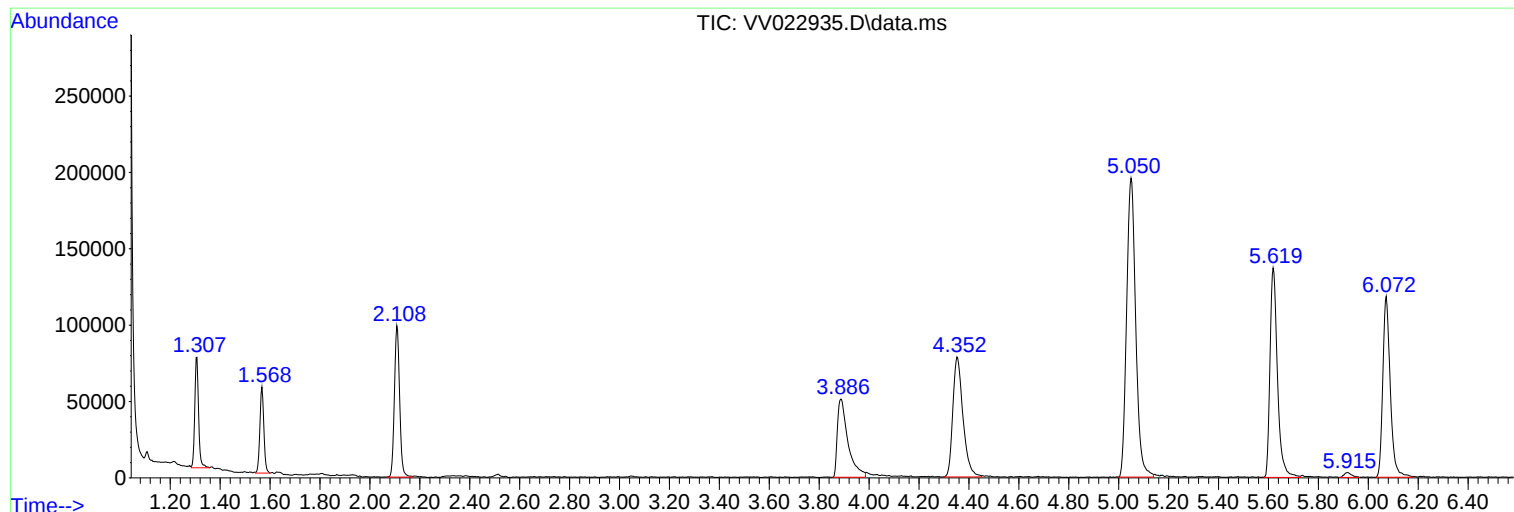

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022935.D
Acq On : 20 Oct 2021 16:30
Operator : SY/MD
Sample : M4246-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022935.D
Acq On : 20 Oct 2021 16:30
Operator : SY/MD
Sample : M4246-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
