

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
 Data File : VV022938.D
 Acq On : 20 Oct 2021 17:42
 Operator : SY/MD
 Sample : M4137-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG91

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	55185	57036	6.83%	1.013%
2	1.568	156	164	177	rBV	43705	47667	5.71%	0.847%
3	2.108	321	332	346	rBV	87850	128123	15.34%	2.275%
4	3.912	876	893	924	rBV3	163650	497111	59.54%	8.829%
5	4.359	1014	1032	1060	rBV2	78585	244162	29.24%	4.336%
6	5.050	1231	1247	1272	rBV2	189730	478212	57.27%	8.493%
7	5.619	1412	1424	1449	rBV	135226	278505	33.36%	4.946%
8	5.918	1505	1517	1537	rBV	66128	137970	16.52%	2.450%
9	6.072	1551	1565	1589	rBV	116607	239612	28.70%	4.256%
10	6.989	1839	1850	1865	rBV	46036	84713	10.15%	1.505%
11	7.317	1940	1952	1964	rBV	212201	371696	44.52%	6.601%
12	7.391	1964	1975	1995	rVB	482217	834965	100.00%	14.829%
13	7.629	2036	2049	2071	rBV	28506	54227	6.49%	0.963%
14	7.976	2137	2157	2181	rBV	307493	539394	64.60%	9.580%
15	8.092	2181	2193	2230	rVV	231759	434281	52.01%	7.713%
16	8.854	2418	2430	2446	rBV	221002	359105	43.01%	6.378%
17	10.217	2844	2854	2873	rBV	82139	130182	15.59%	2.312%
18	10.384	2897	2906	2915	rVB3	18200	28703	3.44%	0.510%
19	11.249	3162	3175	3197	rBV	202580	324501	38.86%	5.763%
20	11.625	3278	3292	3312	rBV	221751	348063	41.69%	6.182%
21	12.252	3475	3487	3498	rVB2	7543	12330	1.48%	0.219%




Sum of corrected areas: 5630558

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022938.D
Acq On : 20 Oct 2021 17:42
Operator : SY/MD
Sample : M4137-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

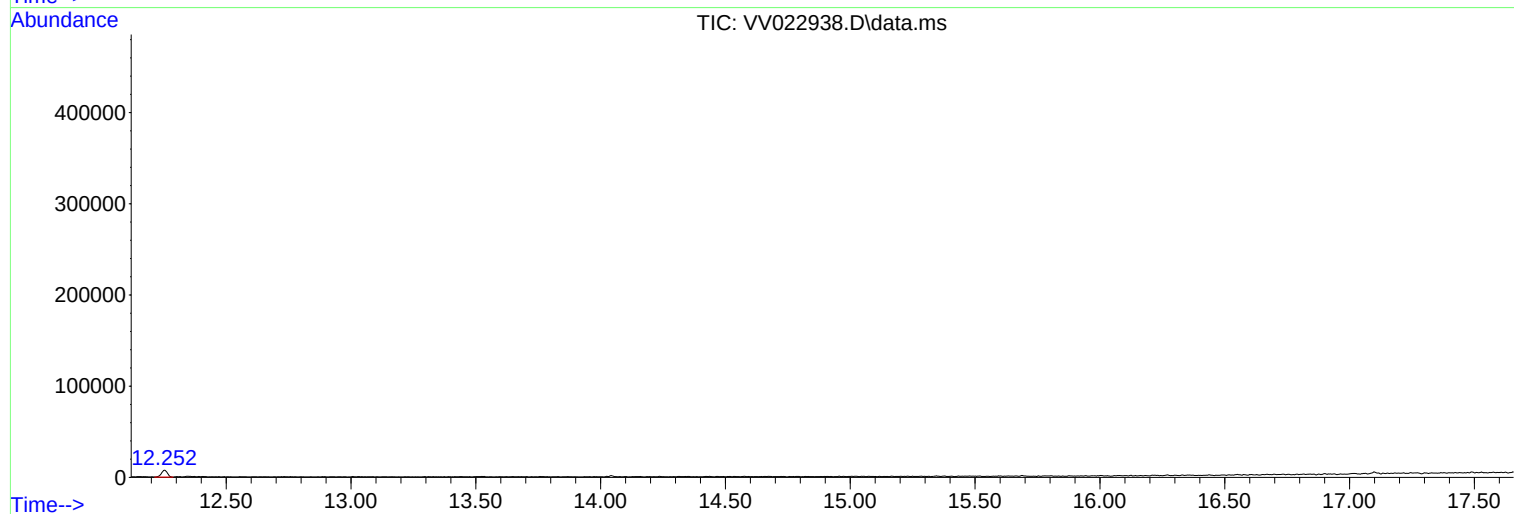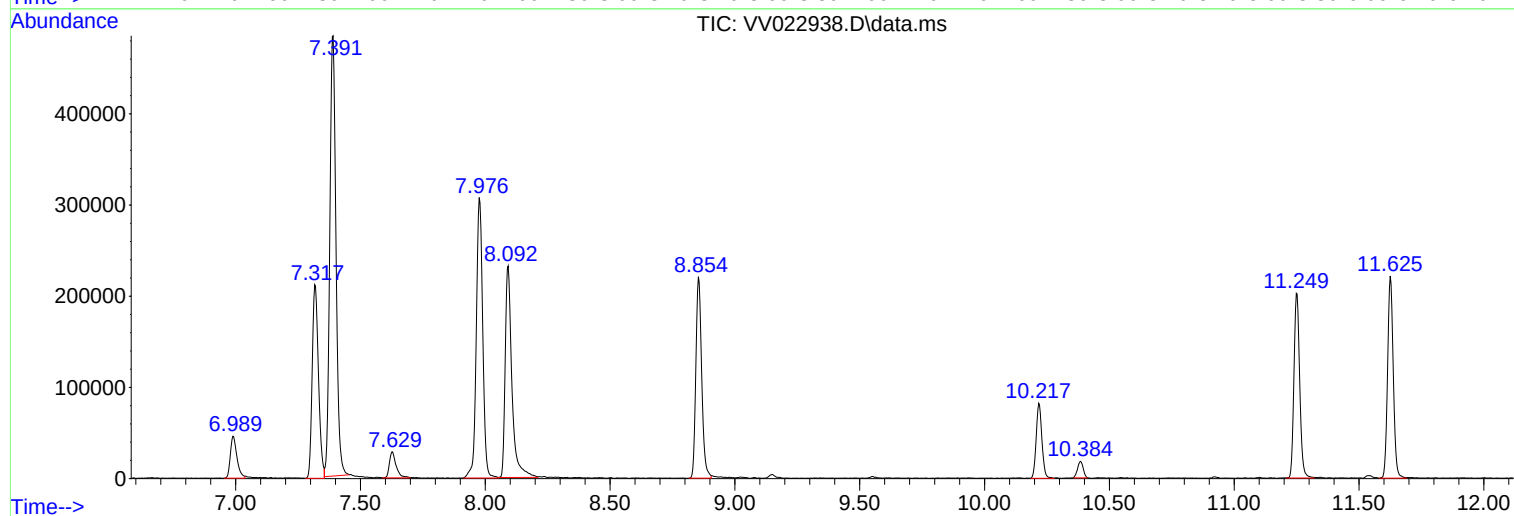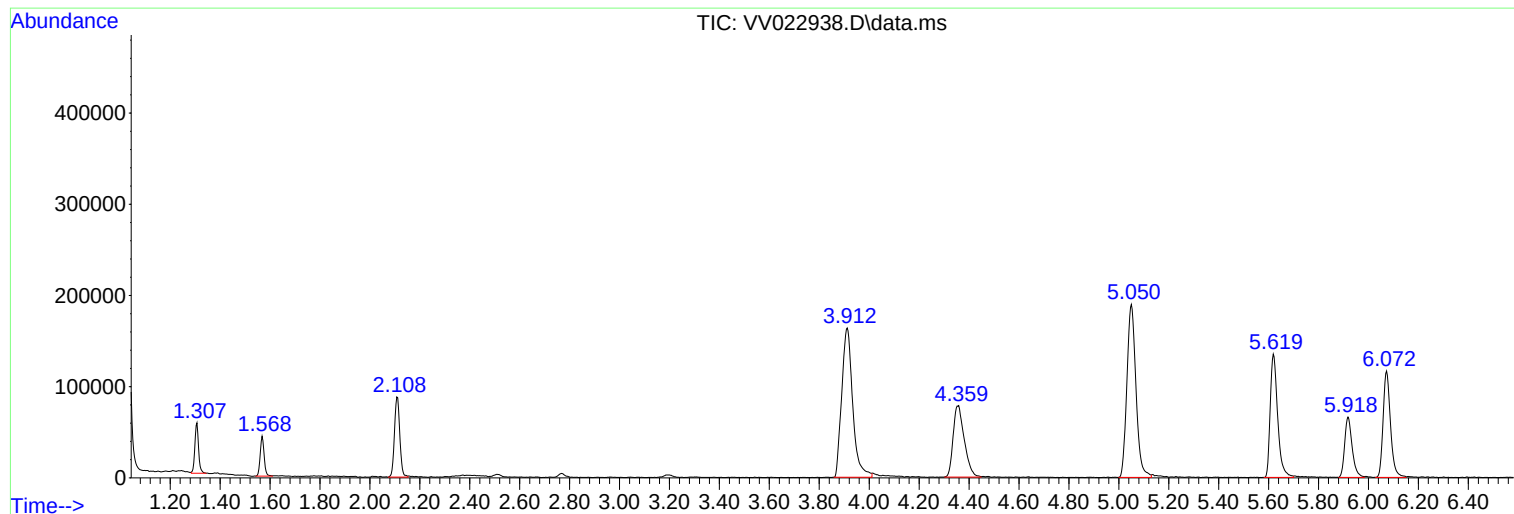

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022938.D
Acq On : 20 Oct 2021 17:42
Operator : SY/MD
Sample : M4137-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022938.D
Acq On : 20 Oct 2021 17:42
Operator : SY/MD
Sample : M4137-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
