

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
 Data File : VV022940.D
 Acq On : 20 Oct 2021 18:29
 Operator : SY/MD
 Sample : M4137-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGA6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB2	69590	74583	15.52%	1.508%
2	1.568	157	164	179	rBV	48300	55064	11.46%	1.114%
3	2.108	320	332	346	rBV2	91077	135105	28.11%	2.732%
4	2.513	448	458	465	rVB6	3233	5489	1.14%	0.111%
5	2.770	523	538	556	rBV3	27408	59162	12.31%	1.196%
6	3.191	654	669	689	rBV	56721	120463	25.07%	2.436%
7	3.291	689	700	712	rVB6	3886	8640	1.80%	0.175%
8	3.912	876	893	927	rBV3	117010	387331	80.60%	7.833%
9	4.355	1012	1031	1059	rBV2	91553	303208	63.09%	6.132%
10	5.050	1231	1247	1268	rBV2	188690	480585	100.00%	9.719%
11	5.619	1412	1424	1446	rBV	132326	271896	56.58%	5.498%
12	5.921	1505	1518	1543	rBV4	38262	82900	17.25%	1.676%
13	6.072	1549	1565	1590	rBV	114941	241359	50.22%	4.881%
14	6.989	1839	1850	1870	rBV	45910	87254	18.16%	1.764%
15	7.320	1940	1953	1966	rBV	210505	376021	78.24%	7.604%
16	7.391	1966	1975	1995	rVB	137174	240440	50.03%	4.862%
17	7.625	2039	2048	2067	rBV2	28823	53125	11.05%	1.074%
18	7.976	2138	2157	2174	rBV2	163226	298447	62.10%	6.035%
19	8.092	2181	2193	2233	rBV	229982	435727	90.67%	8.811%
20	8.854	2420	2430	2454	rBV	216470	356773	74.24%	7.215%
21	9.146	2514	2521	2532	rBV3	5315	9046	1.88%	0.183%
22	10.217	2843	2854	2870	rBV2	84616	133997	27.88%	2.710%
23	10.384	2895	2906	2917	rVB	20364	31762	6.61%	0.642%
24	11.249	3165	3175	3195	rBV	208386	321968	67.00%	6.511%
25	11.538	3254	3265	3278	rBV7	4126	7524	1.57%	0.152%
26	11.625	3278	3292	3309	rBV	225324	353841	73.63%	7.155%
27	12.252	3478	3487	3495	rBV	8368	13322	2.77%	0.269%


Sum of corrected areas: 4945032

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022940.D
Acq On : 20 Oct 2021 18:29
Operator : SY/MD
Sample : M4137-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

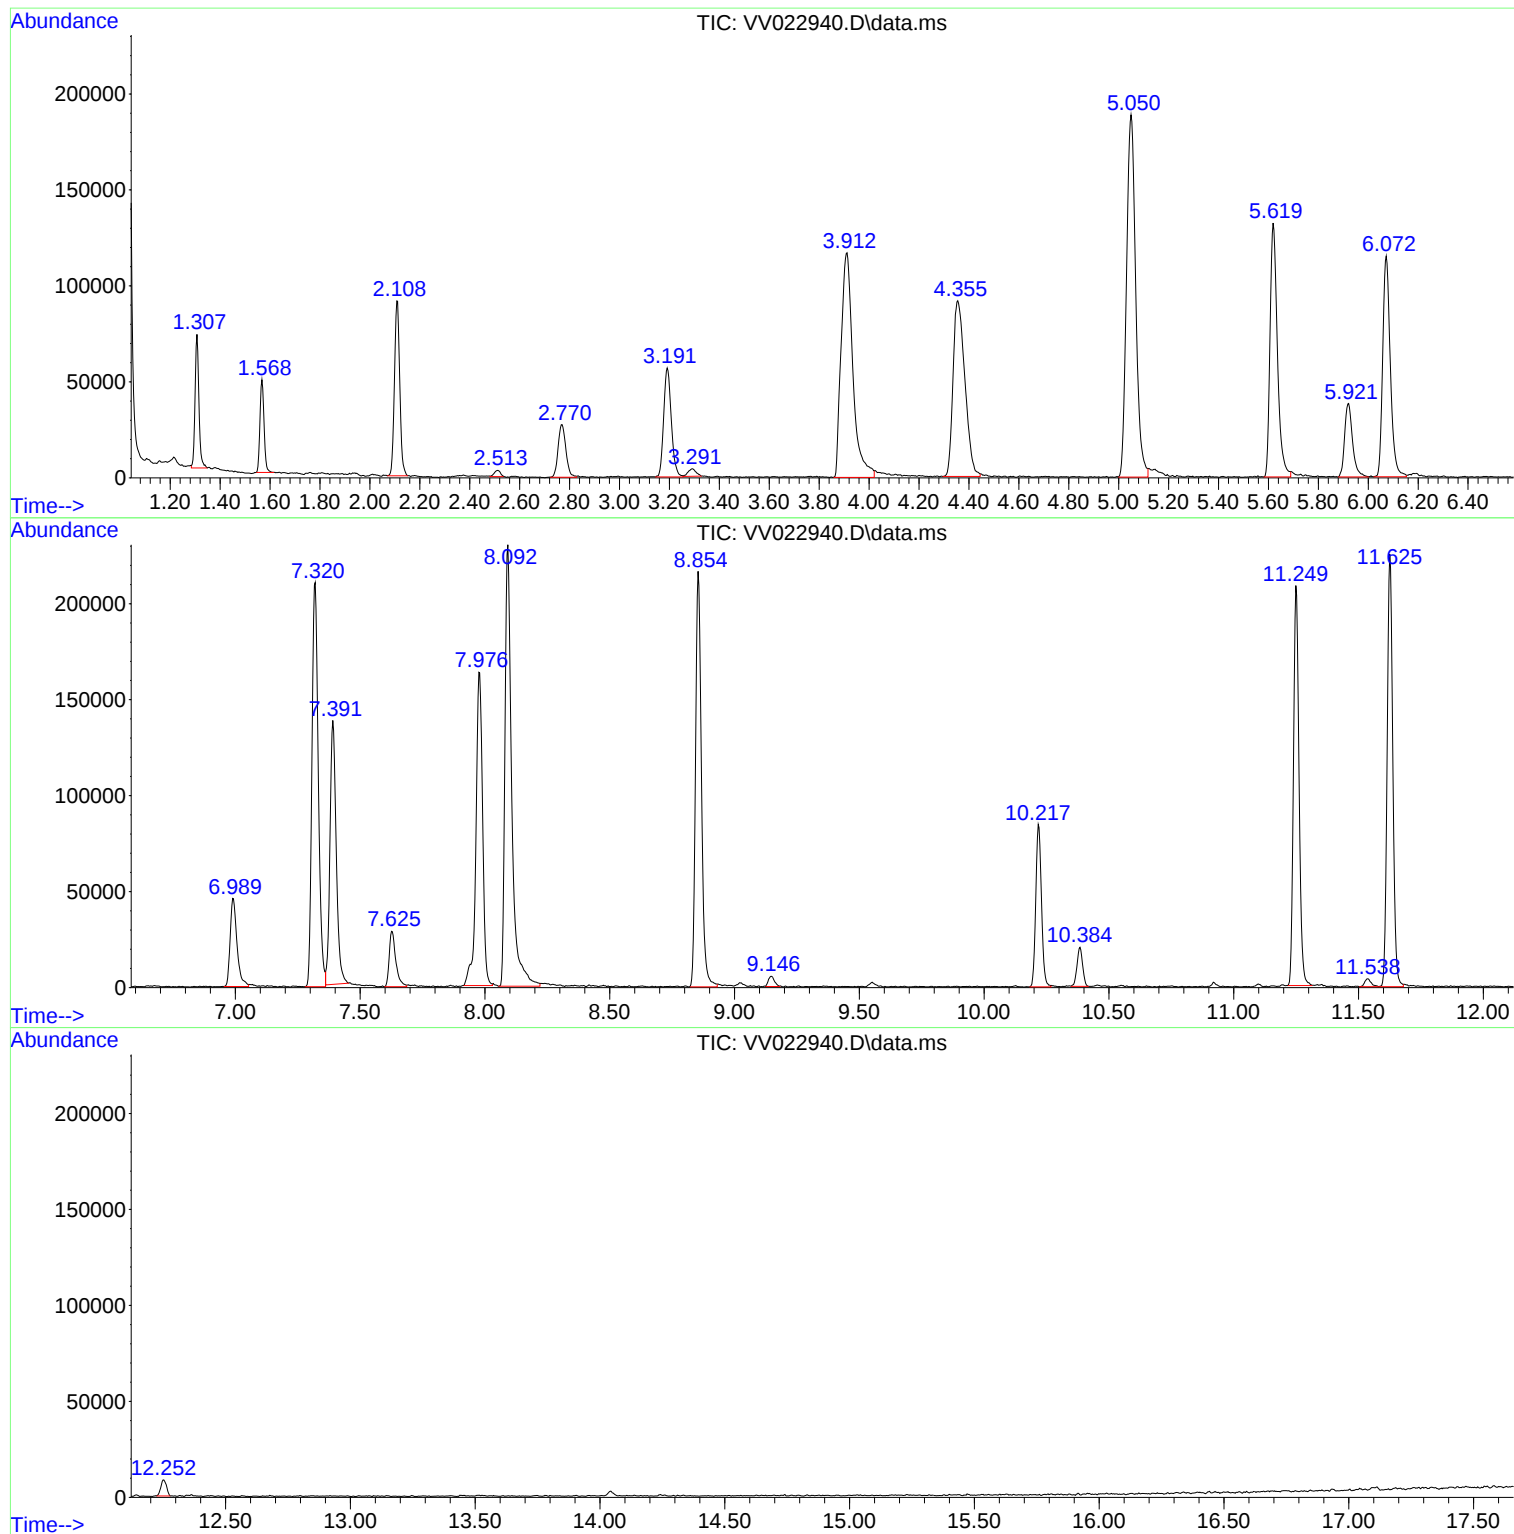

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022940.D
Acq On : 20 Oct 2021 18:29
Operator : SY/MD
Sample : M4137-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022940.D
Acq On : 20 Oct 2021 18:29
Operator : SY/MD
Sample : M4137-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
