

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
 Data File : VV022941.D
 Acq On : 20 Oct 2021 18:53
 Operator : SY/MD
 Sample : M4137-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGC8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	54433	59489	11.95%	1.345%
2	1.568	156	164	173	rBV	43965	52302	10.50%	1.182%
3	2.108	322	332	345	rVV	83560	119958	24.09%	2.711%
4	2.179	345	354	380	rVB	10262	27175	5.46%	0.614%
5	2.510	452	457	467	rVB3	3977	6381	1.28%	0.144%
6	2.770	524	538	557	rVB2	21557	45540	9.14%	1.029%
7	3.195	657	670	684	rBV2	24994	52084	10.46%	1.177%
8	3.912	873	893	922	rBV2	148294	470272	94.43%	10.629%
9	4.352	1014	1030	1058	rBV2	87233	230292	46.24%	5.205%
10	5.050	1227	1247	1278	rBV2	192855	497994	100.00%	11.256%
11	5.619	1413	1424	1450	rBV	134921	284880	57.21%	6.439%
12	5.921	1507	1518	1538	rBV5	13229	30713	6.17%	0.694%
13	6.072	1551	1565	1588	rBV	118343	244776	49.15%	5.532%
14	6.992	1839	1851	1873	rBV	46329	90741	18.22%	2.051%
15	7.317	1939	1952	1970	rBV	215095	387135	77.74%	8.750%
16	7.397	1971	1977	1994	rVB2	9444	20122	4.04%	0.455%
17	7.629	2039	2049	2064	rBV2	27579	49082	9.86%	1.109%
18	7.976	2135	2157	2175	rBV2	60211	115247	23.14%	2.605%
19	8.092	2183	2193	2222	rBV	228022	432223	86.79%	9.769%
20	8.854	2419	2430	2448	rBV	220684	358727	72.03%	8.108%
21	9.146	2513	2521	2529	rBV3	4494	6316	1.27%	0.143%
22	10.217	2843	2854	2870	rBV	86499	135411	27.19%	3.061%
23	10.384	2896	2906	2919	rVB2	10253	17275	3.47%	0.390%
24	11.249	3165	3175	3194	rBV	209117	328041	65.87%	7.414%
25	11.625	3280	3292	3308	rBV	224367	353144	70.91%	7.982%
26	12.249	3475	3486	3496	rBV2	5567	9051	1.82%	0.205%




Sum of corrected areas: 4424371

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022941.D
Acq On : 20 Oct 2021 18:53
Operator : SY/MD
Sample : M4137-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

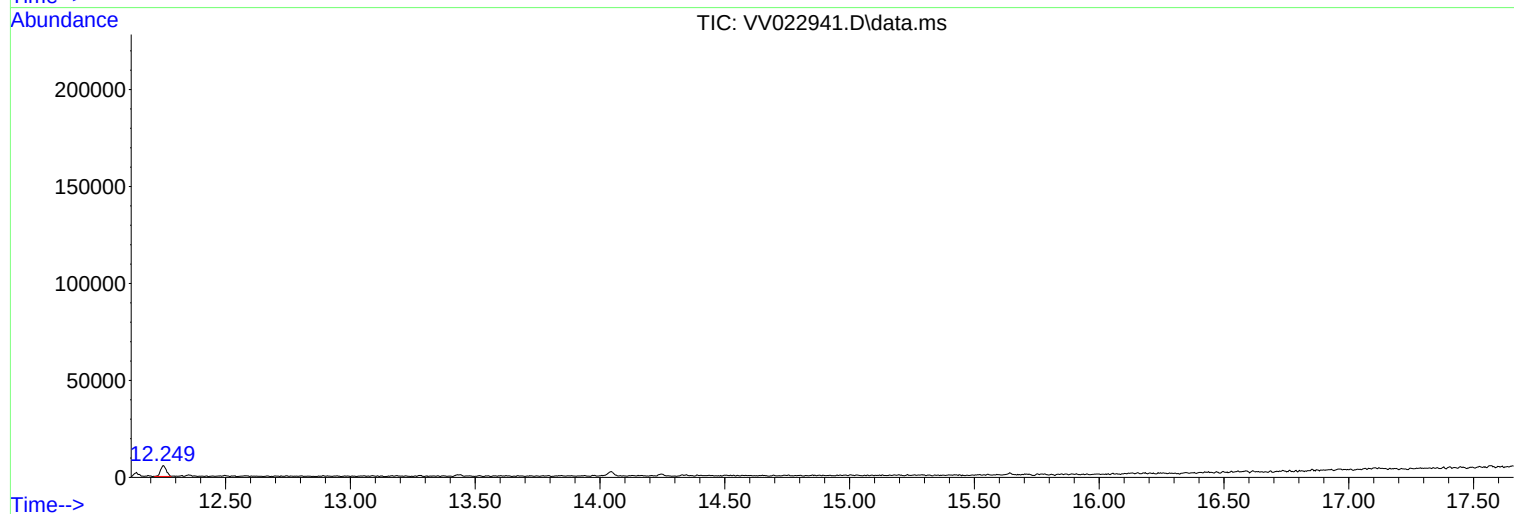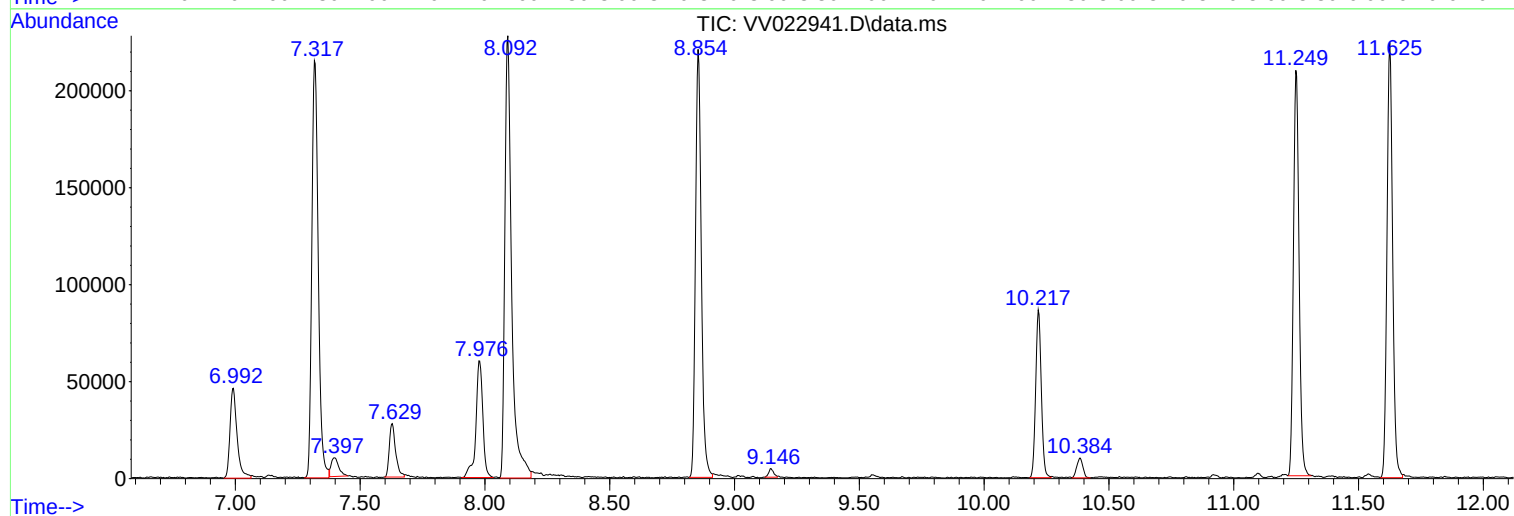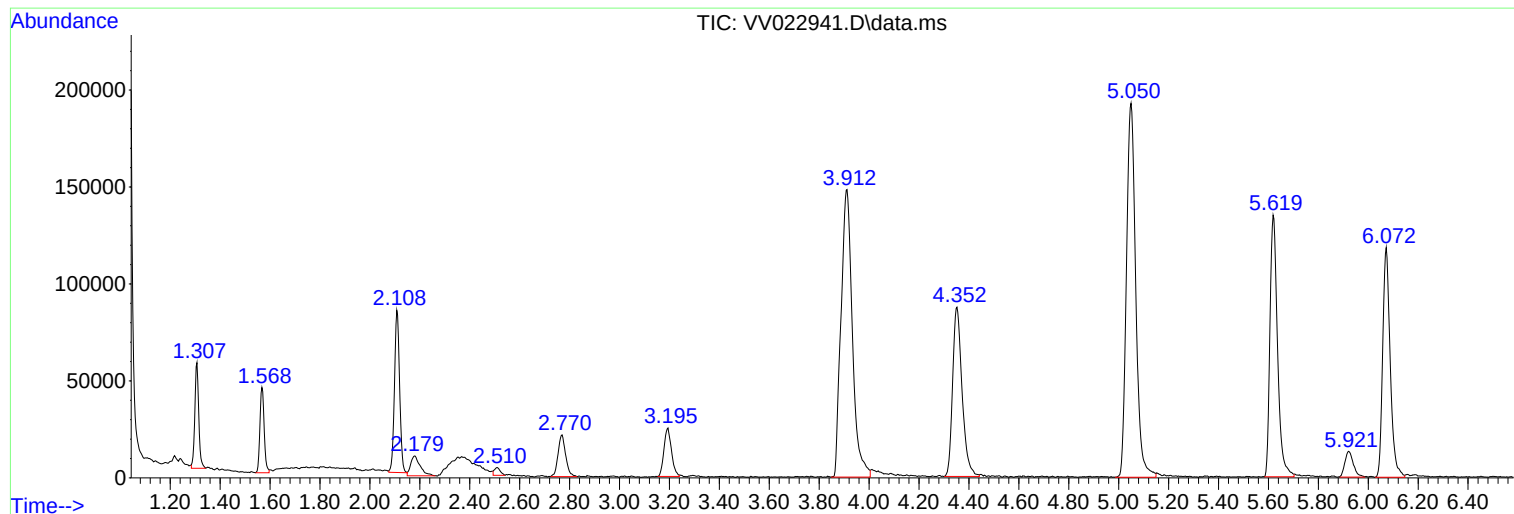

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022941.D
Acq On : 20 Oct 2021 18:53
Operator : SY/MD
Sample : M4137-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
Data File : VV022941.D
Acq On : 20 Oct 2021 18:53
Operator : SY/MD
Sample : M4137-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
