


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102021\
 Data File : VV022926.D
 Acq On : 20 Oct 2021 10:18
 Operator : SY/MD
 Sample : BFB218
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB218

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Oct 22 10:44:34 2021

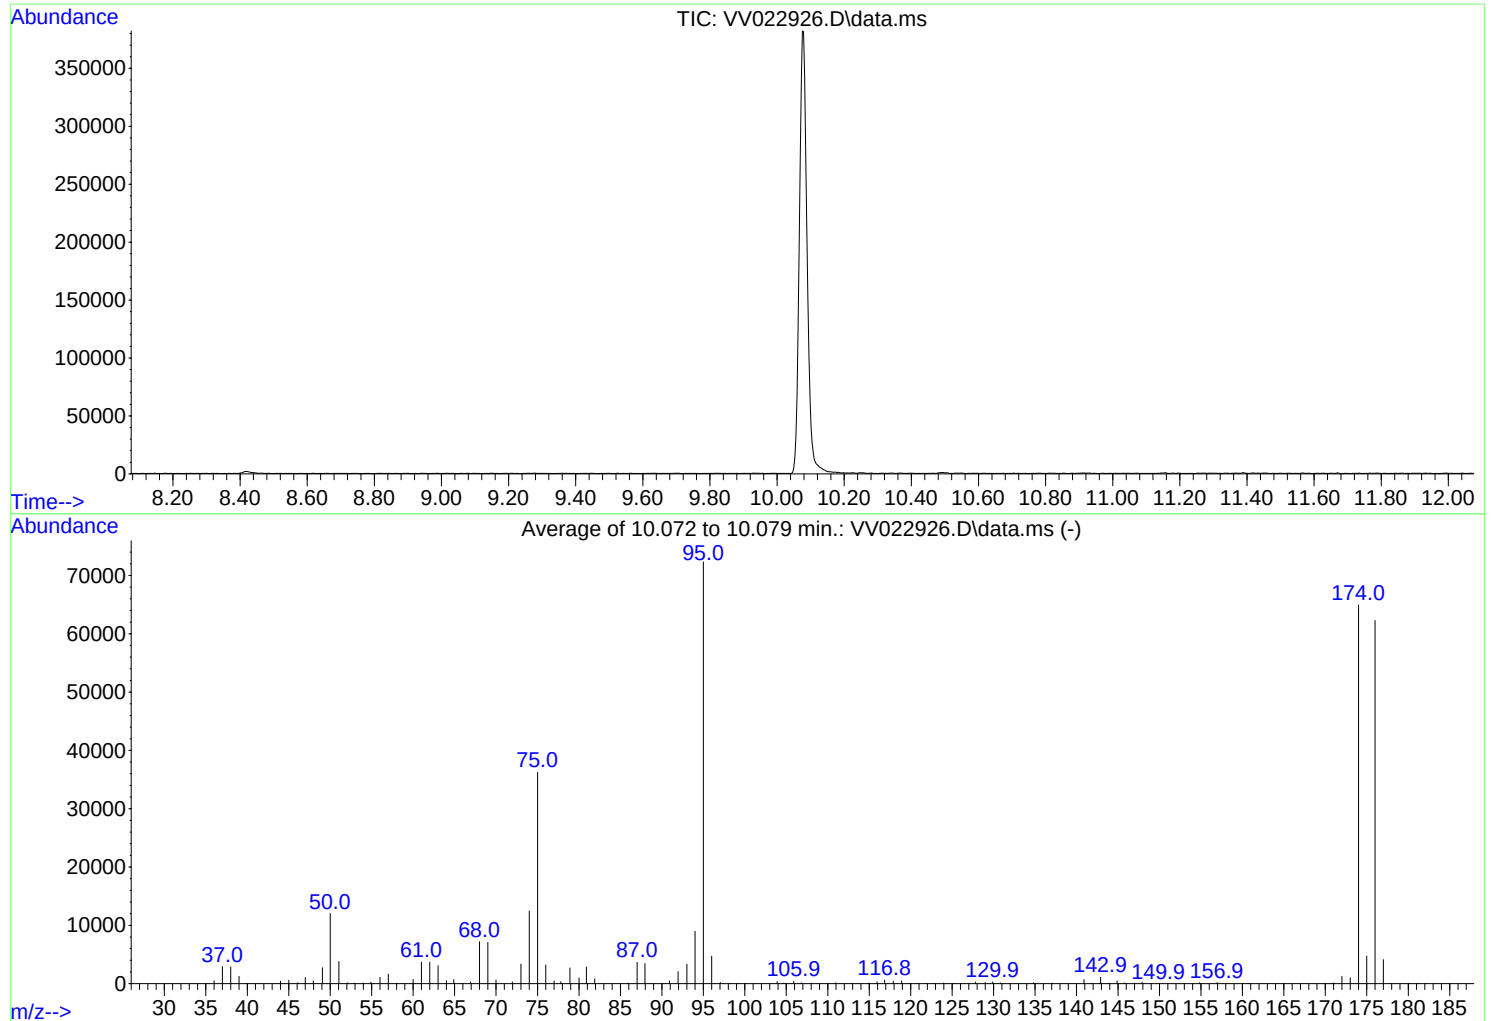

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	12027	PASS
75	95	30	80	50.1	36251	PASS
95	95	100	100	100.0	72344	PASS
96	95	5	9	6.5	4711	PASS
173	174	0.00	2	1.5	992	PASS
174	95	50	120	89.7	64917	PASS
175	174	5	9	7.3	4716	PASS
176	174	95	105	96.0	62309	PASS
177	176	5	10	6.6	4126	PASS

Scan 2798 (10.037 min): VV022926.D\data.ms
BFB218

m/z	Abundance
40.00	189.0
43.90	249.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
36.00	448.0
37.00	2898.0
38.00	2729.0
39.00	1207.0
40.00	225.0
44.10	601.0
45.00	486.0
46.10	178.0
47.00	947.0
47.90	455.0
49.10	2563.0
50.00	11215.0
51.00	3574.0
52.20	123.0
53.00	116.0
54.00	102.0
54.90	214.0
56.00	1061.0
57.00	1585.0
60.00	694.0
61.00	3675.0
62.00	3434.0
63.00	2866.0
64.00	476.0
64.90	636.0
66.90	273.0
68.00	6942.0
69.00	6694.0
70.00	609.0
72.00	283.0
73.00	3230.0
74.00	11721.0
75.00	34216.0
76.00	3092.0
77.00	368.0
77.80	328.0
78.90	2579.0
80.00	884.0
80.90	2644.0
81.90	752.0
85.80	153.0
87.00	3482.0
88.00	3380.0
90.90	366.0
92.00	1873.0
93.00	2960.0
94.00	8352.0
95.00	68056.0
96.00	4547.0
97.10	167.0
103.90	318.0
105.90	414.0
106.80	112.0
110.90	107.0
112.90	105.0
116.00	325.0
116.80	502.0
117.90	428.0
118.90	464.0
124.00	133.0
127.80	269.0
129.00	193.0
129.90	299.0
130.80	101.0
134.80	186.0
137.10	153.0
140.90	658.0
142.90	1050.0
143.90	106.0
144.90	421.0
145.70	139.0
147.90	257.0
154.90	187.0
156.90	195.0
170.80	190.0
172.00	1102.0
173.00	872.0
174.00	59456.0
175.00	4419.0
176.00	56656.0
177.00	3826.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
36.00	498.0
37.00	2997.0
38.00	2955.0
39.00	1299.0
40.00	183.0
44.00	665.0
45.00	581.0
46.10	169.0
47.00	1085.0
48.00	477.0
49.10	2831.0
50.00	12407.0
51.10	3909.0
52.10	134.0
53.90	127.0
54.90	254.0
56.00	1099.0
57.00	1630.0
58.00	117.0
60.00	772.0
61.00	3830.0
62.00	3860.0
63.00	3227.0
64.00	549.0
64.90	705.0
65.90	105.0
66.90	299.0
68.00	7433.0
69.00	7310.0
70.00	647.0
72.00	293.0
73.00	3475.0
74.00	12920.0
75.00	37624.0
76.00	3318.0
77.00	482.0
77.80	363.0
78.90	2759.0
80.00	1050.0
80.90	2934.0
81.90	857.0
85.90	129.0
87.00	3782.0
88.00	3619.0
90.90	483.0
91.90	2156.0
93.00	3433.0
94.00	9351.0
95.00	74848.0
96.00	4851.0
97.00	187.0
103.90	362.0
104.70	143.0
105.90	413.0
106.80	144.0
108.00	114.0
110.90	139.0
114.90	103.0
116.00	358.0
116.90	633.0
117.90	448.0
118.90	471.0
123.90	125.0
127.80	281.0
129.00	231.0
129.90	299.0
130.80	160.0
134.80	184.0
137.10	105.0
140.90	701.0
142.90	1112.0
143.90	108.0
144.90	470.0
145.70	128.0
147.90	261.0
154.90	157.0
156.90	200.0
171.00	182.0
172.00	1273.0
173.00	1011.0
174.00	67336.0
175.00	4835.0
176.00	64440.0
177.00	4241.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
36.00	510.0
37.00	2896.0
38.00	2850.0
39.00	1260.0
39.90	177.0
44.00	695.0
45.00	695.0
46.10	131.0
47.00	1082.0
47.90	441.0
49.00	2790.0
50.00	12459.0
51.10	3897.0
52.00	185.0
52.80	103.0
53.90	116.0
54.90	252.0
56.00	1044.0
57.00	1645.0
58.00	129.0
60.00	719.0
61.00	3557.0
62.00	3711.0
63.00	3155.0
64.00	558.0
64.90	750.0
66.90	268.0
68.00	7223.0
69.00	7233.0
70.00	633.0
71.90	325.0
73.00	3376.0
74.00	12743.0
75.00	36912.0
76.00	3148.0
77.00	576.0
77.80	319.0
78.90	2719.0
80.00	1069.0
80.90	2986.0
81.90	835.0
87.00	3715.0
87.90	3396.0
90.90	552.0
92.00	2183.0
93.00	3539.0
94.00	9229.0
95.00	74128.0
96.00	4736.0
97.00	209.0
103.90	367.0
104.70	160.0
105.90	393.0
106.80	142.0
108.10	123.0
111.00	148.0
114.90	119.0
115.90	327.0
116.90	678.0
117.90	378.0
118.90	484.0
123.90	118.0
127.80	310.0
129.00	195.0
129.90	289.0
130.80	192.0
134.80	165.0
140.90	721.0
141.80	101.0
142.90	1103.0
144.90	523.0
145.80	130.0
147.90	221.0
149.90	118.0
154.80	148.0
157.00	202.0
160.80	111.0
171.10	162.0
172.00	1412.0
173.00	1094.0
174.00	67960.0
175.00	4895.0
176.00	65832.0
177.00	4311.0
177.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218