
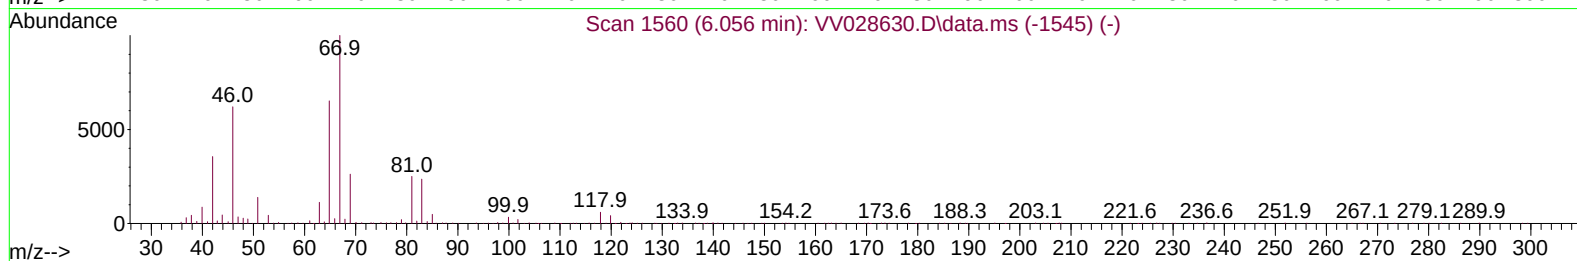
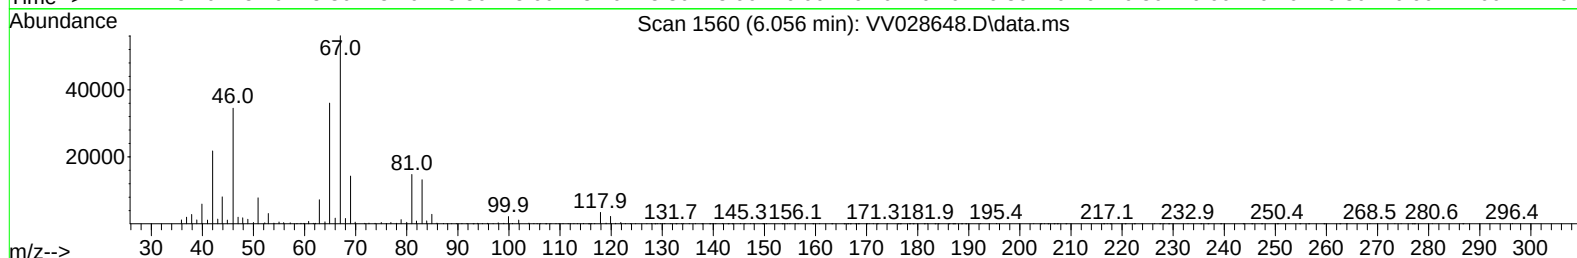


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028648.D
Acq On : 20 Oct 2022 20:37
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Oct 21 01:14:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 21 00:53:32 2022
Response via : Initial Calibration

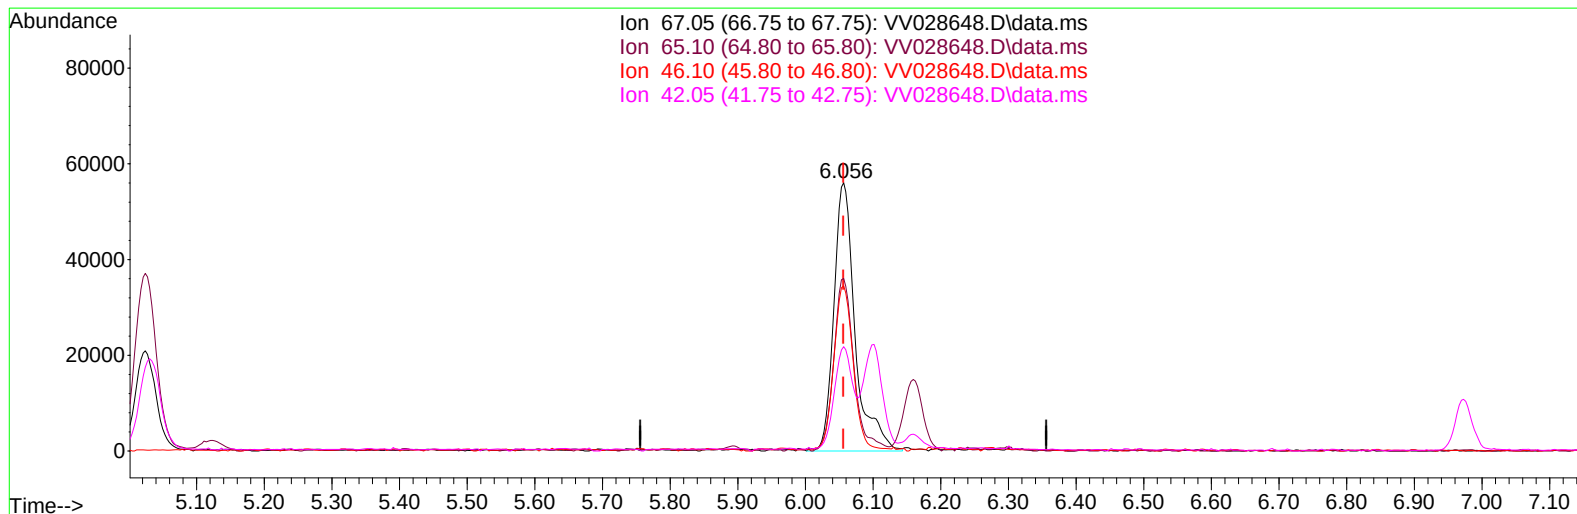

TIC: VV028648.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

6.056min (+ 0.000) 6.32 ug/L

response 122831

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	65.70	61.05
46.10	59.70	55.07
42.05	36.70	32.34