

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
 Data File : VV028634.D
 Acq On : 20 Oct 2022 14:44
 Operator : SY/MD
 Sample : VV1020WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK253

Quant Time: Oct 21 01:10:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 21 00:53:32 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.603	114	221545	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	145350	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	62636	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.294	65	121839	5.555	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	111.000%	
7) Chloroethane-d5	1.558	69	95693	5.550	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	111.000%	
11) 1,1-Dichloroethene-d2	2.095	63	167374	4.391	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	87.800%	
20) 2-Butanone-d5	3.950	46	219607	53.195	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	106.400%	
24) Chloroform-d	4.336	84	175252	5.387	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	107.800%	
26) 1,2-Dichloroethane-d4	5.024	65	97006	5.505	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	110.000%	
32) Benzene-d6	5.031	84	381870	6.038	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	120.800%	
36) 1,2-Dichloropropane-d6	6.056	67	126513	6.380	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	127.600%	
41) Toluene-d8	7.301	98	280155	6.125	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	122.600%	
43) trans-1,3-Dichloroprop...	7.613	79	28059	5.829	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	116.600%	
46) 2-Hexanone-d5	8.104	63	95902	47.980	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.960%	
56) 1,1,2,2-Tetrachloroeth...	10.211	84	49874	5.325	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	106.400%	
66) 1,2-Dichlorobenzene-d4	11.616	152	65630	5.829	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	116.600%	
Target Compounds						
16) Methylene chloride	2.497	84	7570	0.367	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028634.D
Acq On : 20 Oct 2022 14:44
Operator : SY/MD
Sample : VV1020WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK253

Quant Time: Oct 21 01:10:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 21 00:53:32 2022
Response via : Initial Calibration

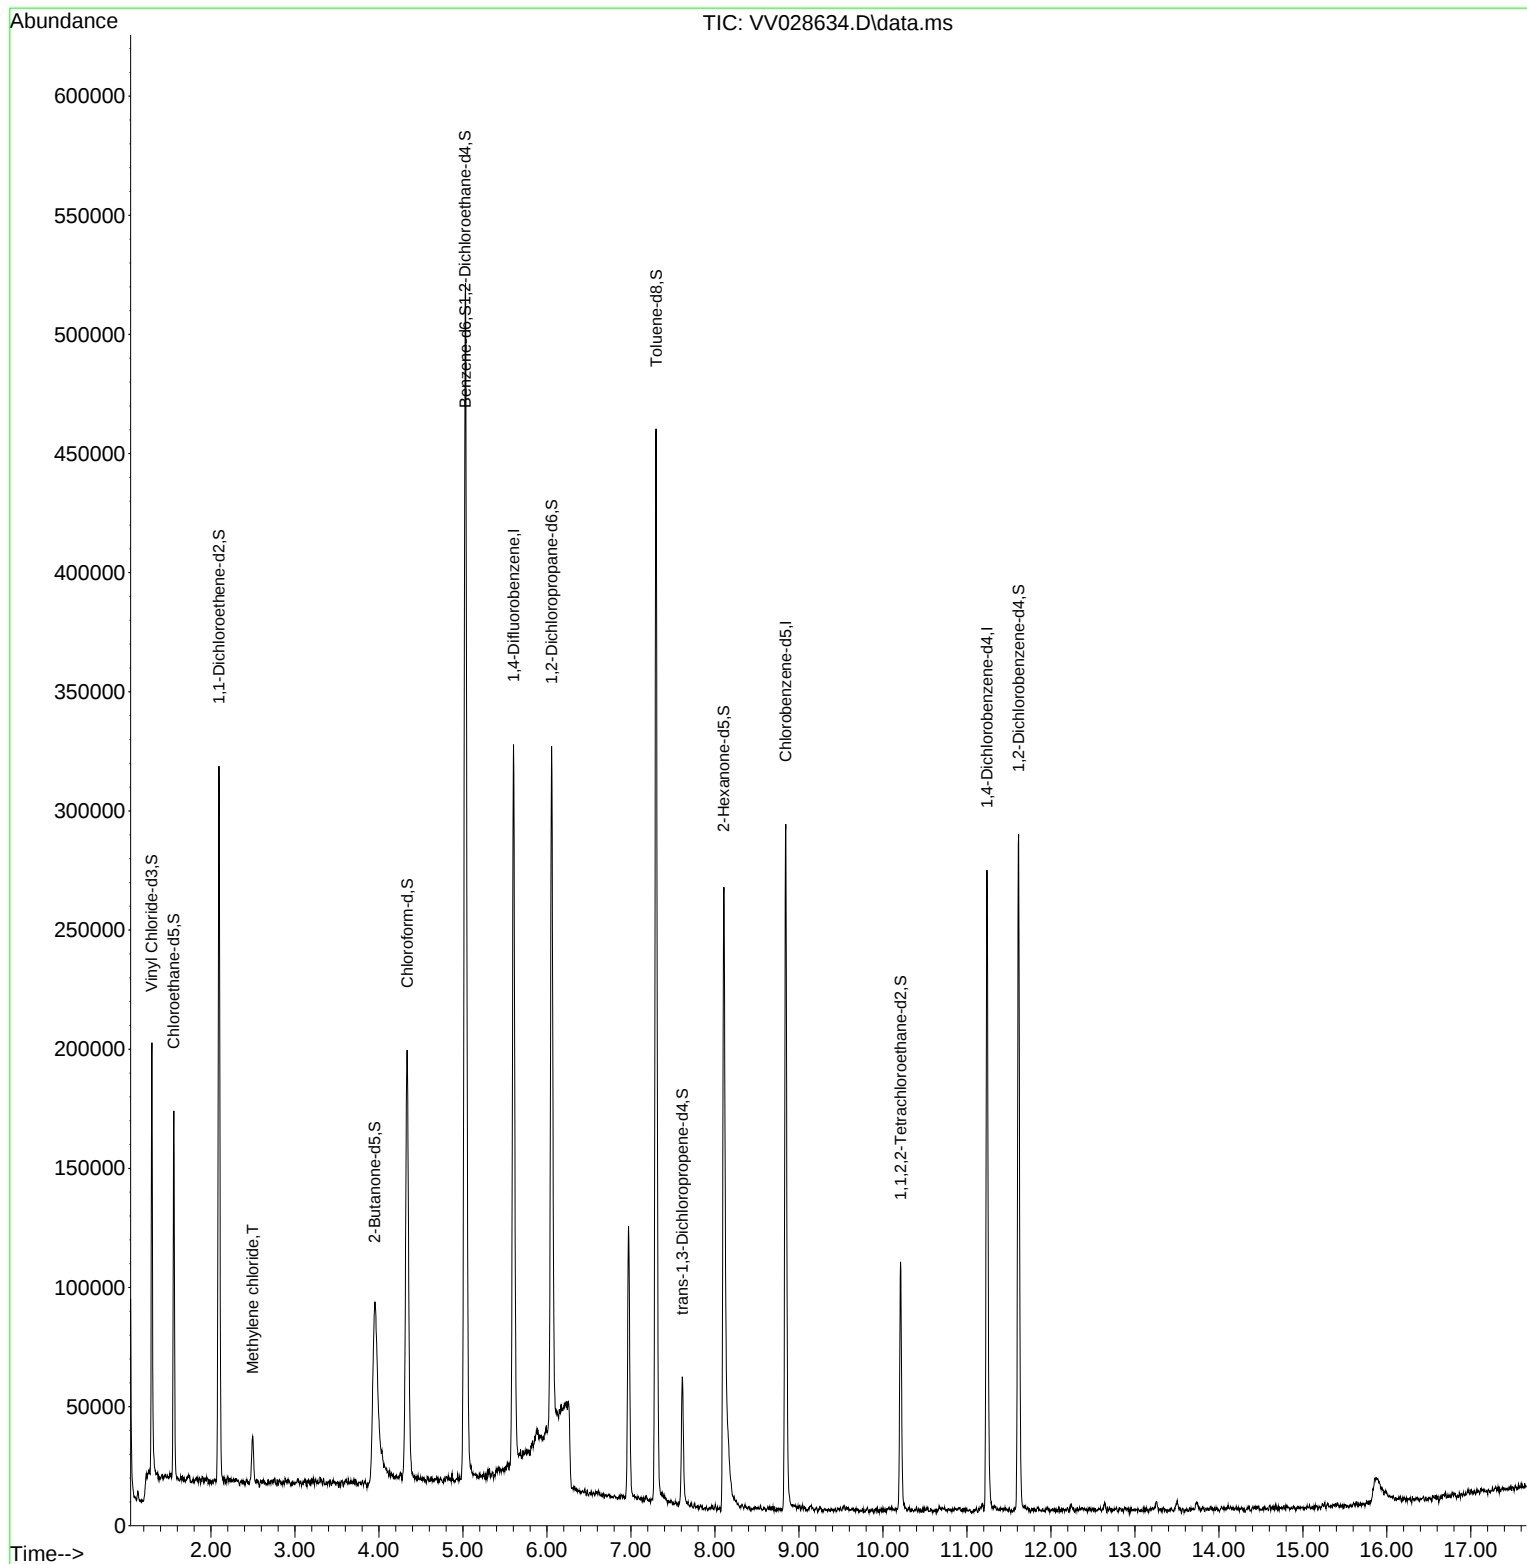

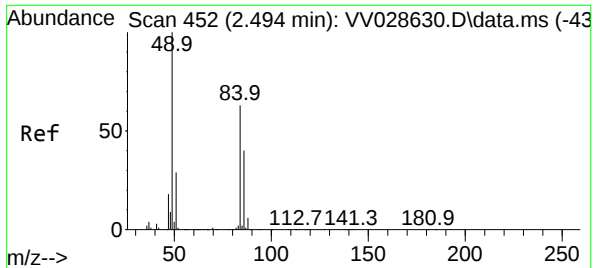

#16
Methylene chloride
Concen: 0.367 ug/L
RT: 2.497 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV028634.D
Acq: 20 Oct 2022 14:44

Instrument :
MSVOA_V
ClientSampleId :
VBLK253

Tgt Ion: 84 Resp: 7570
Ion Ratio Lower Upper
84 100
86 66.5 44.4 82.4
49 163.0 110.8 205.8

