

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
 Data File : VV028634.D
 Acq On : 20 Oct 2022 14:44
 Operator : SY/MD
 Sample : VV1020WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK253

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.230	49	59	61	rBV9	11650	15084	1.37%	0.216%
2	1.298	73	80	95	rVB	181242	186643	16.98%	2.670%
3	1.558	154	161	173	rVB	154727	172505	15.69%	2.468%
4	2.095	319	328	342	rBV	299621	422668	38.44%	6.046%
5	2.497	445	453	464	rVB2	19688	32273	2.94%	0.462%
6	3.954	888	906	929	rBV	74141	296151	26.94%	4.236%
7	4.336	1010	1025	1043	rVB	177965	433598	39.44%	6.202%
8	5.031	1225	1241	1260	rBV2	501880	1099472	100.00%	15.728%
9	5.603	1406	1419	1437	rBV	302498	586397	53.33%	8.388%
10	6.056	1549	1560	1575	rBV	282429	536277	48.78%	7.671%
11	6.973	1833	1845	1858	rBV	114199	197441	17.96%	2.824%
12	7.301	1934	1947	1965	rBV	449607	773708	70.37%	11.068%
13	7.613	2033	2044	2062	rVB3	53329	92196	8.39%	1.319%
14	8.108	2186	2198	2235	rBV2	262129	604388	54.97%	8.646%
15	8.844	2413	2427	2447	rBV	288145	481027	43.75%	6.881%
16	10.211	2840	2852	2866	rBV	103872	164608	14.97%	2.355%
17	11.239	3160	3172	3191	rBV	269045	429285	39.04%	6.141%
18	11.616	3276	3289	3306	rBV	283289	453662	41.26%	6.490%
19	15.860	4598	4609	4611	rBV	8268	13322	1.21%	0.191%




Sum of corrected areas: 6990705

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028634.D
Acq On : 20 Oct 2022 14:44
Operator : SY/MD
Sample : VV1020WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

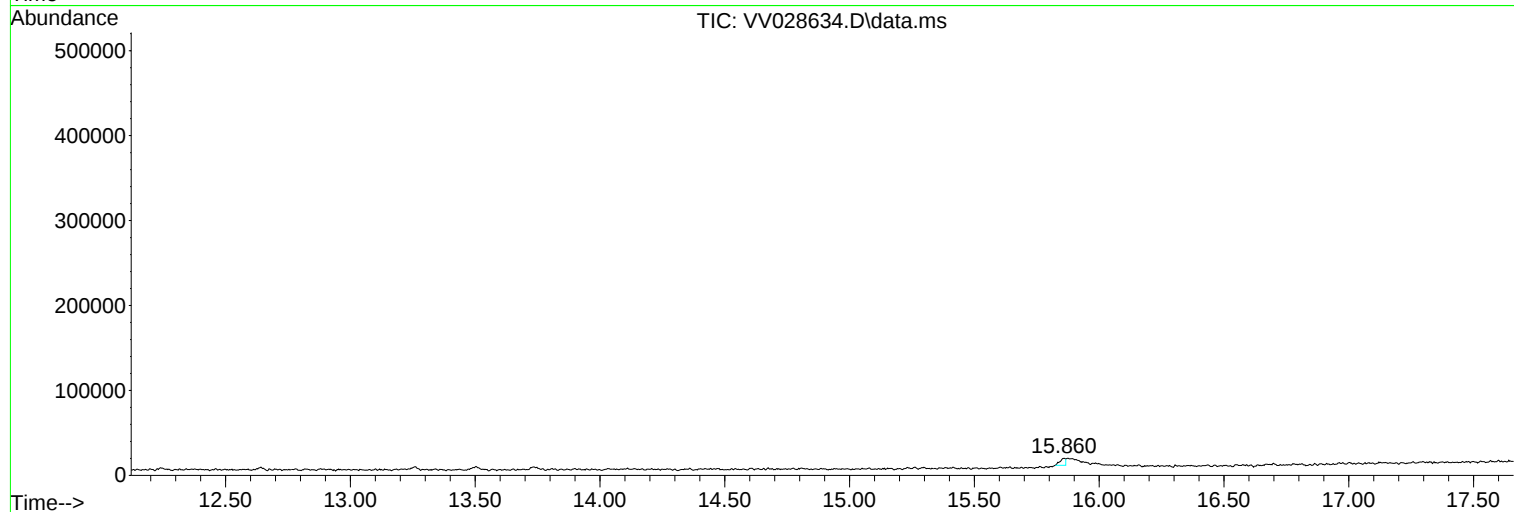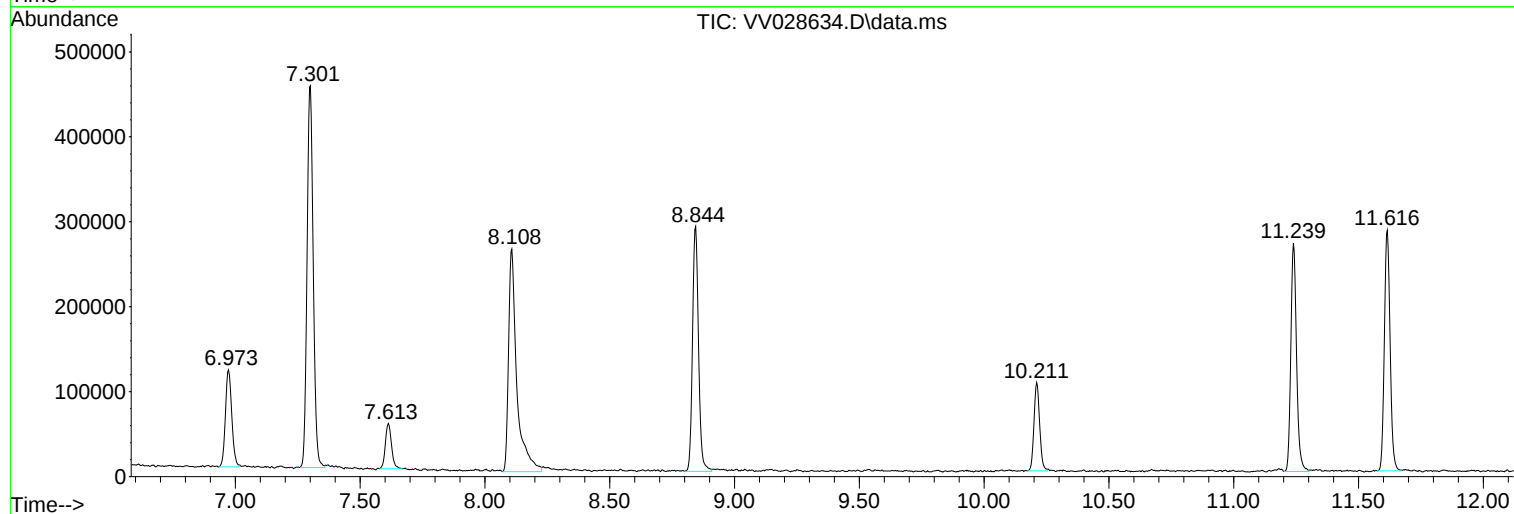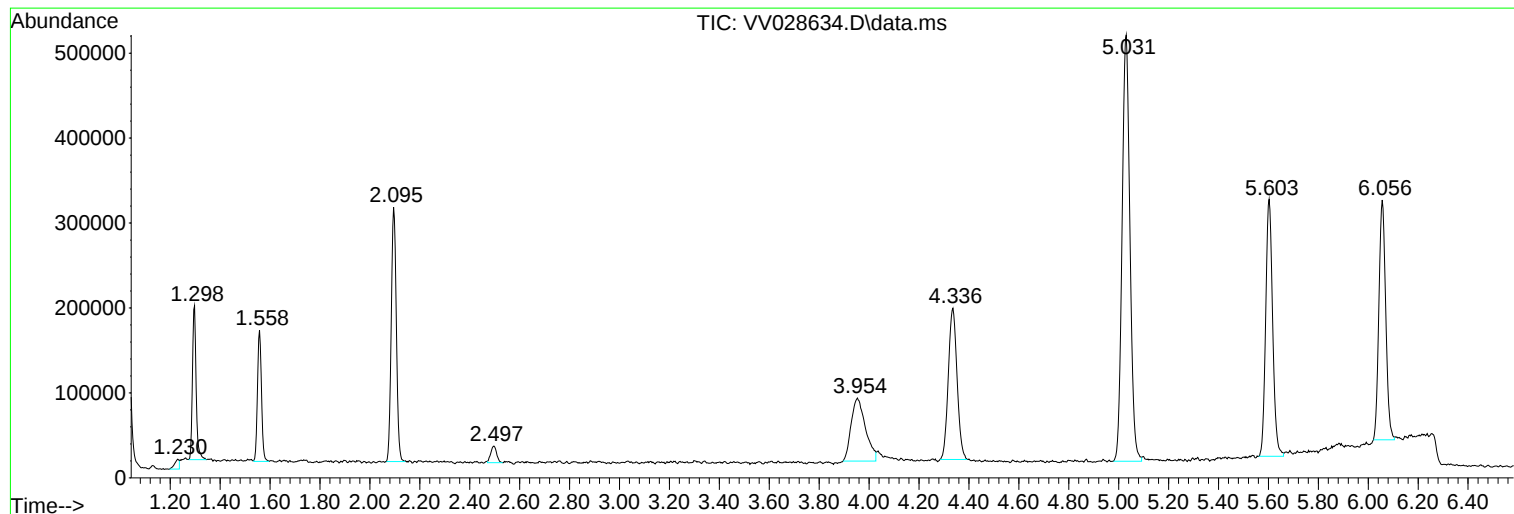

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028634.D
Acq On : 20 Oct 2022 14:44
Operator : SY/MD
Sample : VV1020WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028634.D
Acq On : 20 Oct 2022 14:44
Operator : SY/MD
Sample : VV1020WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc