

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
 Data File : VV028635.D
 Acq On : 20 Oct 2022 15:18
 Operator : SY/MD
 Sample : N5173-03DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXS8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.233	49	60	63	rBV9	12090	18816	2.17%	0.335%
2	1.301	75	81	89	rBV	81428	82992	9.58%	1.478%
3	1.574	160	166	177	rVB	90734	100828	11.63%	1.796%
4	2.111	325	333	345	rVB	151817	216778	25.01%	3.861%
5	2.510	449	457	467	rVB	48342	75271	8.69%	1.341%
6	3.976	898	913	935	rVB2	57692	206618	23.84%	3.680%
7	4.349	1016	1029	1048	rVB	138137	340607	39.30%	6.067%
8	5.037	1230	1243	1269	rVB3	374578	866627	100.00%	15.436%
9	5.616	1410	1423	1442	rBV	186388	382628	44.15%	6.815%
10	5.911	1501	1515	1532	rBV	198934	396254	45.72%	7.058%
11	6.075	1552	1566	1587	rBV	138510	284771	32.86%	5.072%
12	6.995	1843	1852	1866	rBV	51119	90351	10.43%	1.609%
13	7.320	1939	1953	1971	rBV	214214	377456	43.55%	6.723%
14	7.632	2040	2050	2066	rBV2	26369	50134	5.78%	0.893%
15	7.976	2144	2157	2169	rBV3	74189	126505	14.60%	2.253%
16	8.108	2186	2198	2233	rBV2	262769	593387	68.47%	10.569%
17	8.850	2418	2429	2449	rBV	284134	468099	54.01%	8.338%
18	10.214	2842	2853	2865	rBV	96304	150734	17.39%	2.685%
19	11.242	3162	3173	3193	rBV	262730	420643	48.54%	7.492%
20	11.615	3277	3289	3301	rBV	219834	349542	40.33%	6.226%
21	15.847	4593	4605	4607	rBV10	10334	15309	1.77%	0.273%




Sum of corrected areas: 5614350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028635.D
Acq On : 20 Oct 2022 15:18
Operator : SY/MD
Sample : N5173-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

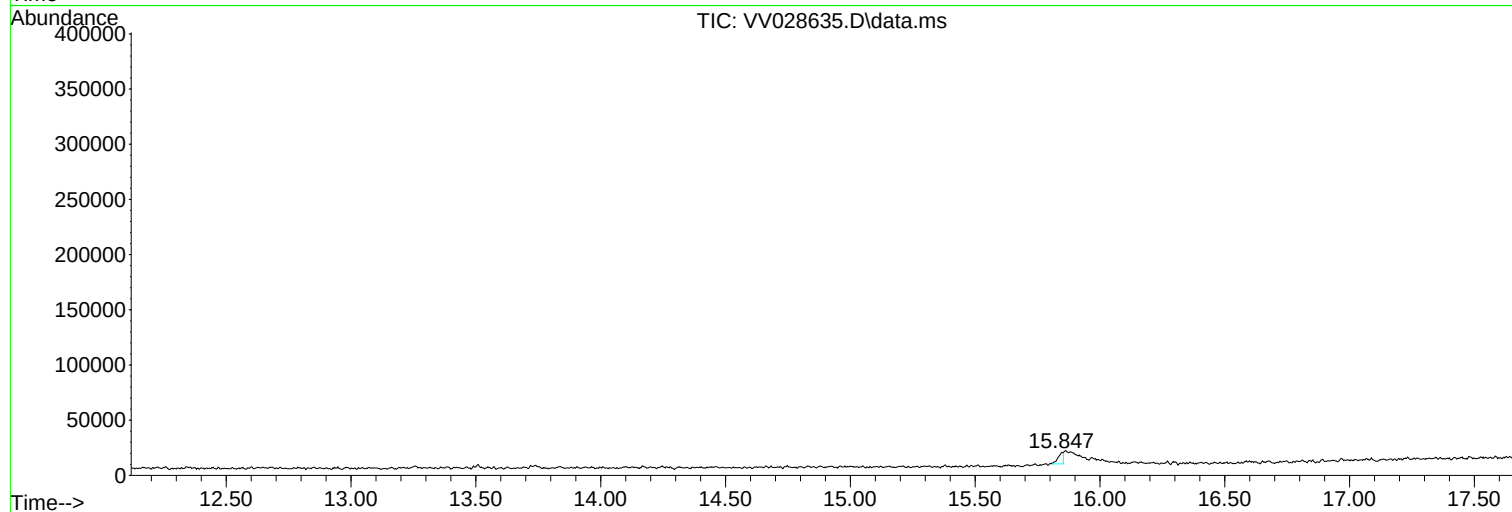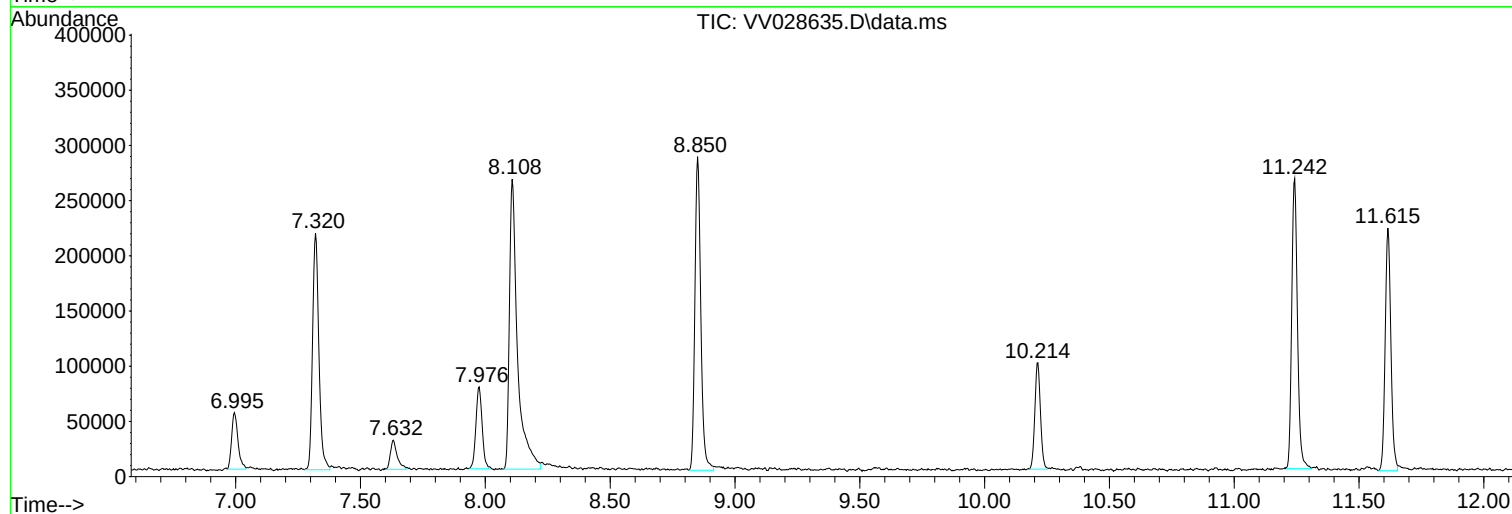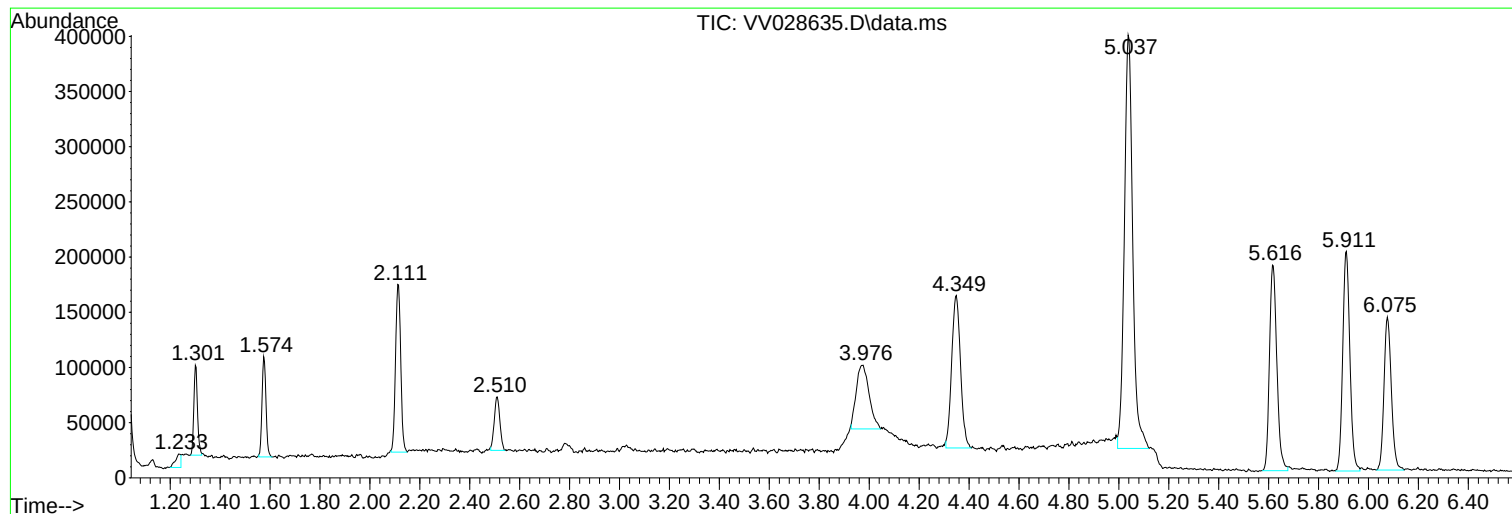

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028635.D
Acq On : 20 Oct 2022 15:18
Operator : SY/MD
Sample : N5173-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028635.D
Acq On : 20 Oct 2022 15:18
Operator : SY/MD
Sample : N5173-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc