

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
 Data File : VV028636.D
 Acq On : 20 Oct 2022 15:42
 Operator : SY/MD
 Sample : N5173-02DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXS7DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028636.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	21	27	41	rVB2	32474	37017	3.88%	0.471%
2	1.233	48	60	67	rBV7	13768	32600	3.42%	0.415%
3	1.294	73	79	97	rVB	158424	170669	17.91%	2.171%
4	1.558	153	161	173	rVB	134042	151916	15.94%	1.932%
5	2.095	318	328	342	rBV	260079	369714	38.79%	4.702%
6	2.494	443	452	462	rBV	33799	53127	5.57%	0.676%
7	3.950	880	905	927	rBV2	63842	291995	30.64%	3.714%
8	4.336	1011	1025	1044	rVB	159300	387967	40.71%	4.935%
9	5.031	1226	1241	1263	rBV2	437213	953017	100.00%	12.122%
10	5.603	1407	1419	1439	rBV	299743	582747	61.15%	7.412%
11	5.892	1496	1509	1526	rBV	430024	815308	85.55%	10.370%
12	6.056	1549	1560	1574	rBV	242233	469517	49.27%	5.972%
13	6.973	1834	1845	1860	rBV	95490	169976	17.84%	2.162%
14	7.297	1934	1946	1961	rBV	390142	661541	69.42%	8.414%
15	7.612	2032	2044	2058	rBV2	37705	65748	6.90%	0.836%
16	7.960	2137	2152	2165	rBV	404014	676031	70.94%	8.598%
17	8.108	2185	2198	2229	rBV2	230815	512593	53.79%	6.520%
18	8.844	2416	2427	2451	rBV	293716	475907	49.94%	6.053%
19	10.210	2840	2852	2866	rVB	90599	147596	15.49%	1.877%
20	11.239	3160	3172	3193	rBV	266782	421886	44.27%	5.366%
21	11.616	3277	3289	3305	rBV	242954	392221	41.16%	4.989%
22	15.866	4593	4611	4613	rBV	10700	23110	2.42%	0.294%




Sum of corrected areas: 7862203

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028636.D
Acq On : 20 Oct 2022 15:42
Operator : SY/MD
Sample : N5173-02DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

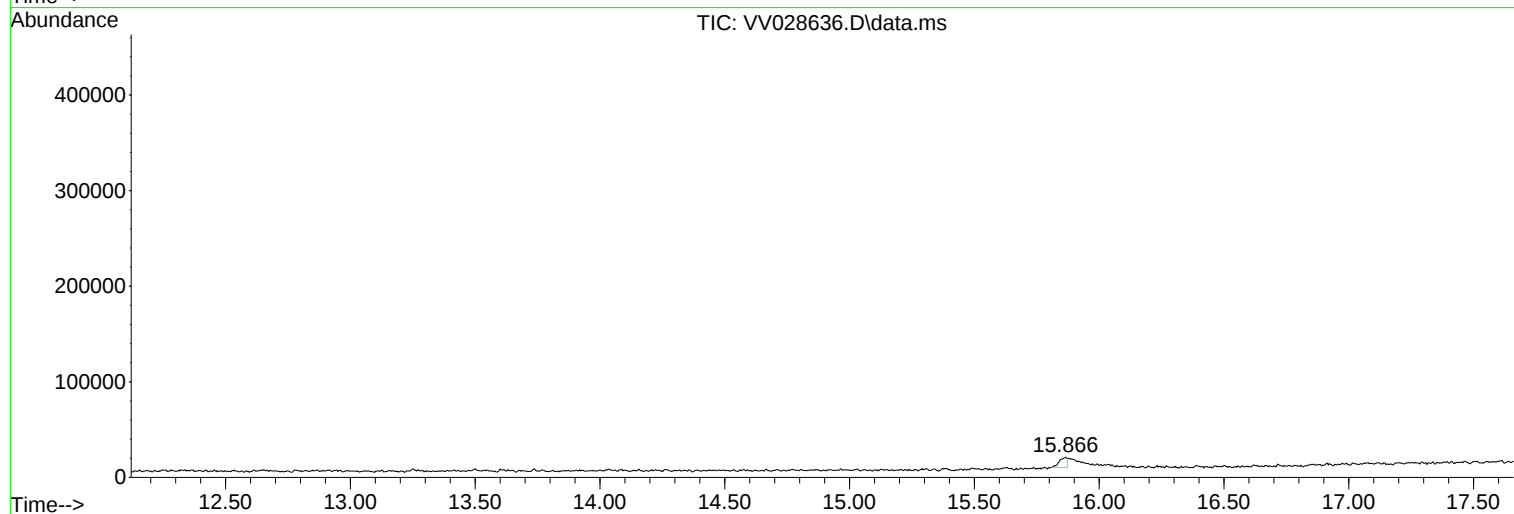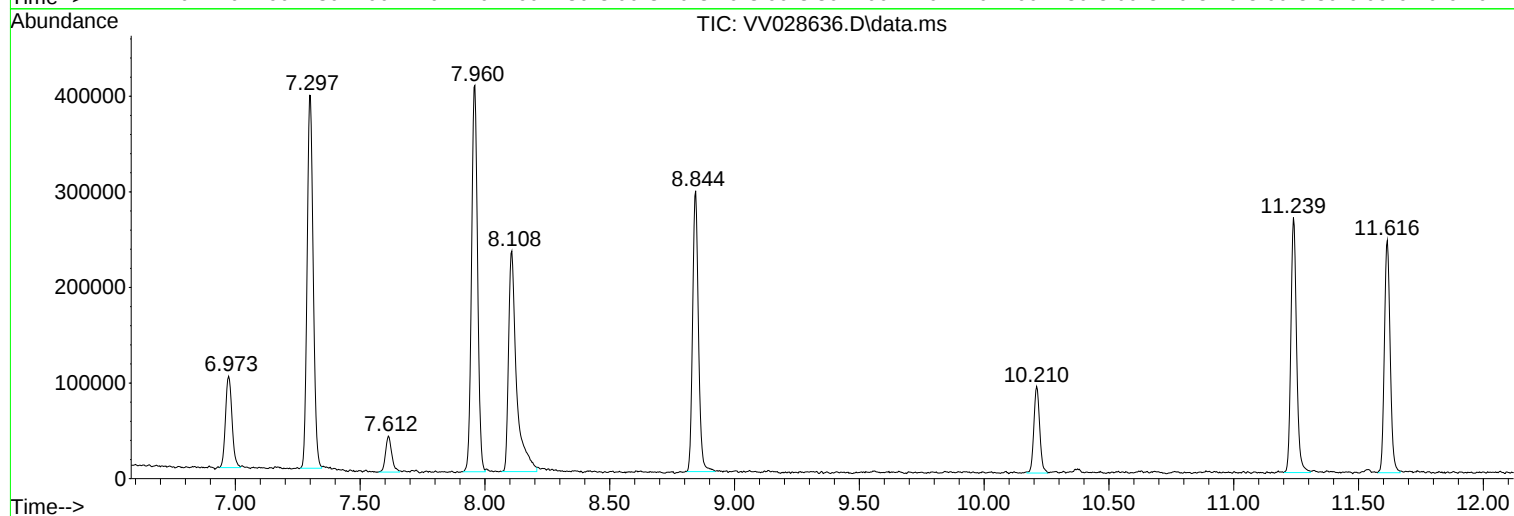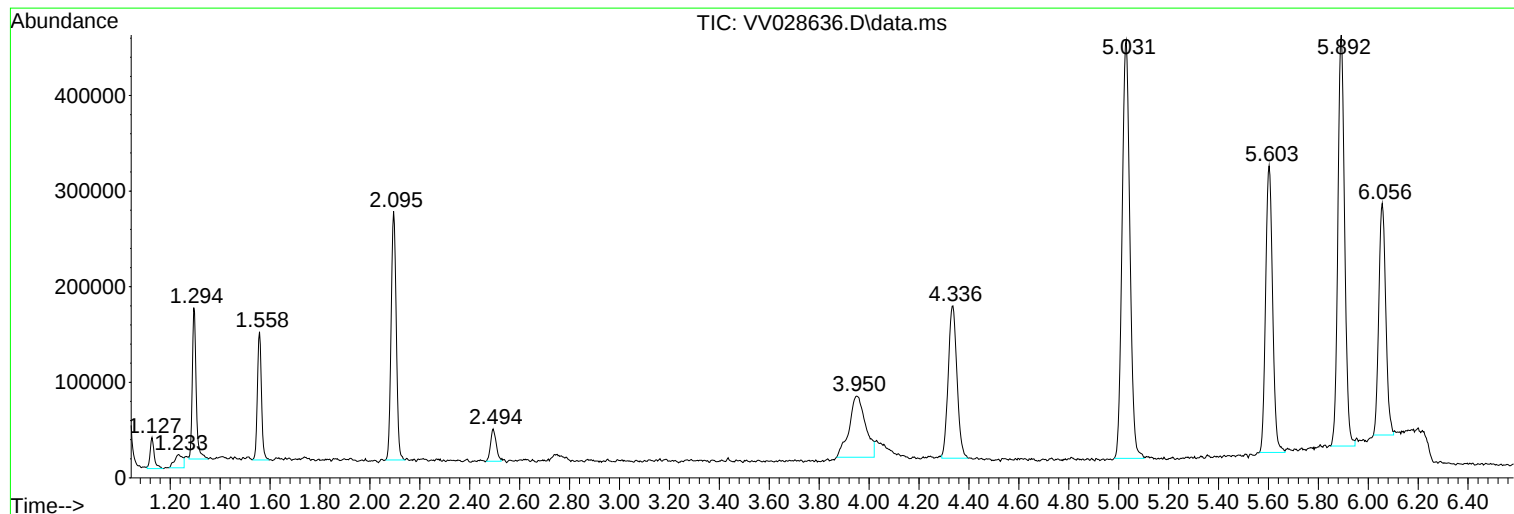

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028636.D
Acq On : 20 Oct 2022 15:42
Operator : SY/MD
Sample : N5173-02DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028636.D
Acq On : 20 Oct 2022 15:42
Operator : SY/MD
Sample : N5173-02DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc