

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
 Data File : VV028637.D
 Acq On : 20 Oct 2022 16:07
 Operator : SY/MD
 Sample : N5173-04DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXS9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.233	48	60	61	rBV10	11730	16065	1.75%	0.241%
2	1.297	73	80	95	rBV	150276	158221	17.24%	2.378%
3	1.561	155	162	171	rBV	127509	145496	15.85%	2.187%
4	1.748	215	220	228	rVB2	13917	17137	1.87%	0.258%
5	2.101	320	330	345	rVB	256281	361760	39.41%	5.437%
6	2.500	446	454	464	rVB	44231	67356	7.34%	1.012%
7	3.905	878	891	892	rBV4	18757	32997	3.59%	0.496%
8	4.336	1011	1025	1042	rVB	156045	375853	40.95%	5.649%
9	5.030	1226	1241	1263	rVB2	415562	917888	100.00%	13.796%
10	5.606	1408	1420	1435	rBV	292258	562180	61.25%	8.450%
11	5.895	1499	1510	1525	rVB	268495	503201	54.82%	7.563%
12	6.063	1551	1562	1575	rBV	229632	443831	48.35%	6.671%
13	6.982	1837	1848	1862	rBV	66732	120136	13.09%	1.806%
14	7.307	1936	1949	1967	rBV	310363	538617	58.68%	8.096%
15	7.619	2035	2046	2063	rBV2	35685	65653	7.15%	0.987%
16	7.966	2139	2154	2168	rBV	235633	390434	42.54%	5.868%
17	8.111	2188	2199	2233	rBV2	220675	502677	54.76%	7.555%
18	8.847	2417	2428	2444	rBV	288724	469312	51.13%	7.054%
19	10.210	2843	2852	2863	rBV	88329	140541	15.31%	2.112%
20	11.242	3161	3173	3189	rBV	260088	412761	44.97%	6.204%
21	11.615	3275	3289	3303	rBV	239535	380128	41.41%	5.713%
22	15.860	4594	4609	4612	rBV	14647	30990	3.38%	0.466%




Sum of corrected areas: 6653234

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028637.D
Acq On : 20 Oct 2022 16:07
Operator : SY/MD
Sample : N5173-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

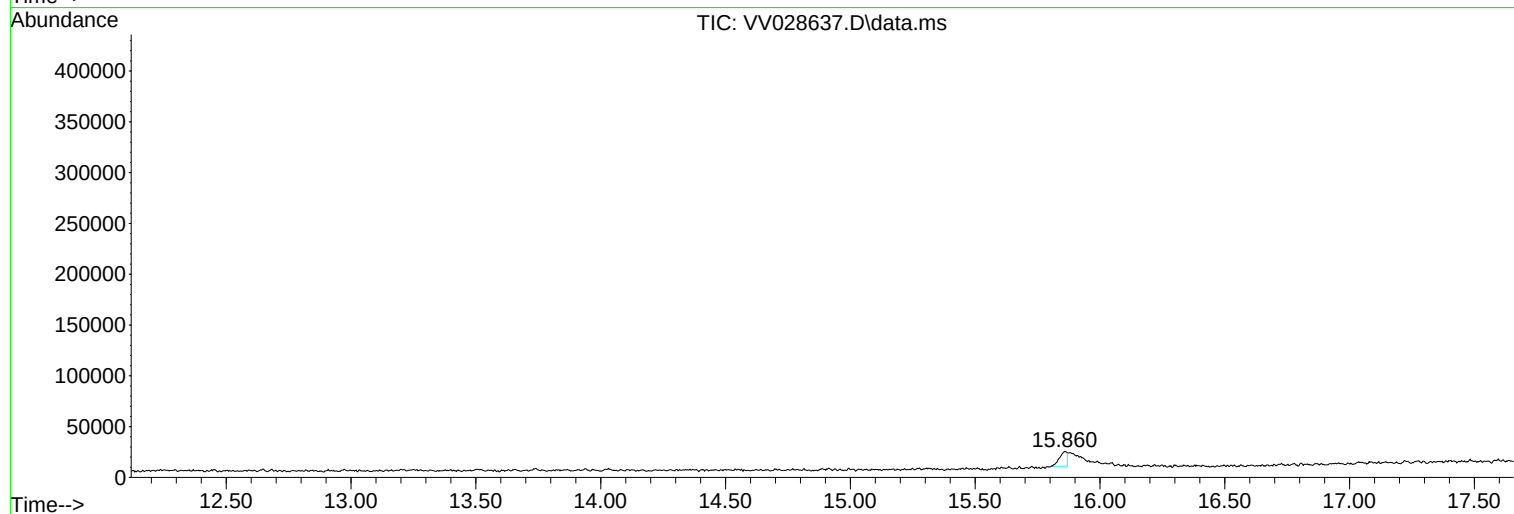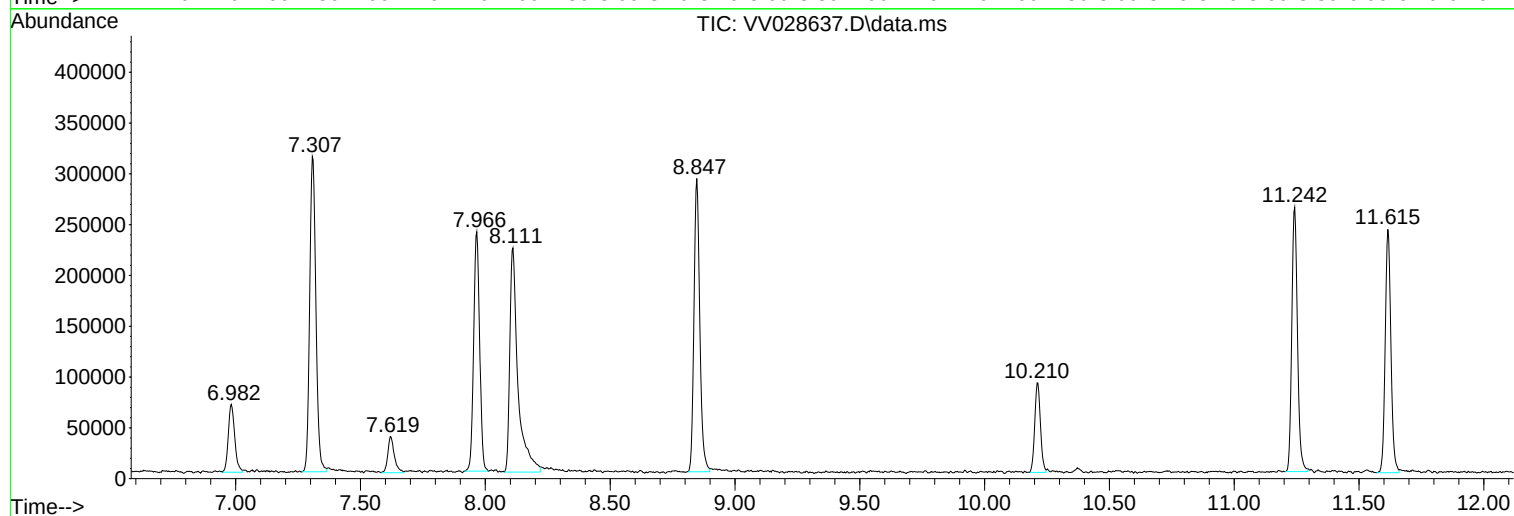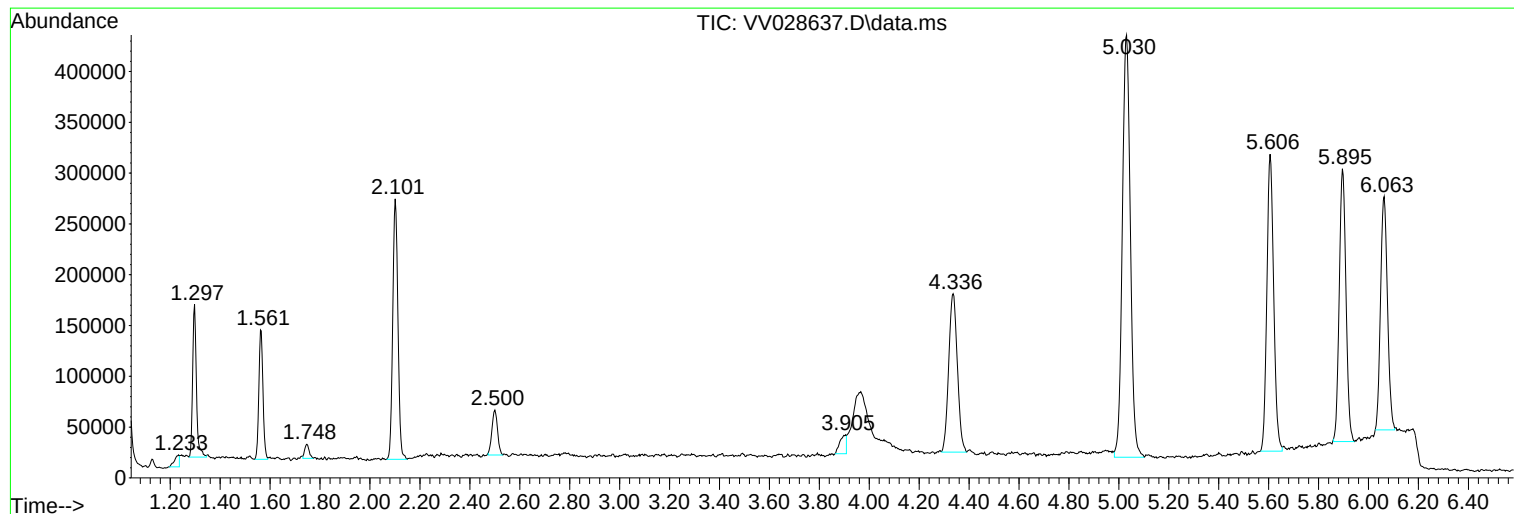

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028637.D
Acq On : 20 Oct 2022 16:07
Operator : SY/MD
Sample : N5173-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028637.D
Acq On : 20 Oct 2022 16:07
Operator : SY/MD
Sample : N5173-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc