

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
 Data File : VV028638.D
 Acq On : 20 Oct 2022 16:32
 Operator : SY/MD
 Sample : N5173-05DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXTODL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	73	79	97	rVB	150338	162196	17.83%	2.380%
2	1.558	153	161	172	rBV	134620	148145	16.29%	2.174%
3	1.741	210	218	227	rVB	43098	55184	6.07%	0.810%
4	2.095	318	328	342	rVB2	254161	362471	39.85%	5.318%
5	2.494	443	452	462	rBV	47007	75433	8.29%	1.107%
6	3.947	878	904	926	rBV2	66874	304550	33.48%	4.468%
7	4.333	1011	1024	1043	rVB2	149807	360705	39.66%	5.292%
8	5.031	1226	1241	1263	rBV2	417752	909516	100.00%	13.344%
9	5.603	1408	1419	1433	rBV	293187	553907	60.90%	8.127%
10	5.892	1497	1509	1523	rBV	193165	358415	39.41%	5.259%
11	6.056	1549	1560	1577	rBV	238411	459676	50.54%	6.744%
12	6.973	1835	1845	1862	rBV	65549	115755	12.73%	1.698%
13	7.297	1935	1946	1964	rBV	302936	521229	57.31%	7.647%
14	7.613	2032	2044	2057	rBV2	35146	62166	6.84%	0.912%
15	7.960	2137	2152	2166	rBV	254792	426365	46.88%	6.256%
16	8.104	2186	2197	2227	rBV2	224916	508329	55.89%	7.458%
17	8.841	2413	2426	2444	rBV	287817	472234	51.92%	6.929%
18	10.211	2839	2852	2869	rBV	89538	144485	15.89%	2.120%
19	11.239	3160	3172	3189	rBV	262899	417630	45.92%	6.127%
20	11.616	3276	3289	3303	rBV	235720	379263	41.70%	5.565%
21	15.863	4596	4610	4611	rBV	11078	18028	1.98%	0.265%




Sum of corrected areas: 6815682

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028638.D
Acq On : 20 Oct 2022 16:32
Operator : SY/MD
Sample : N5173-05DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXT0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

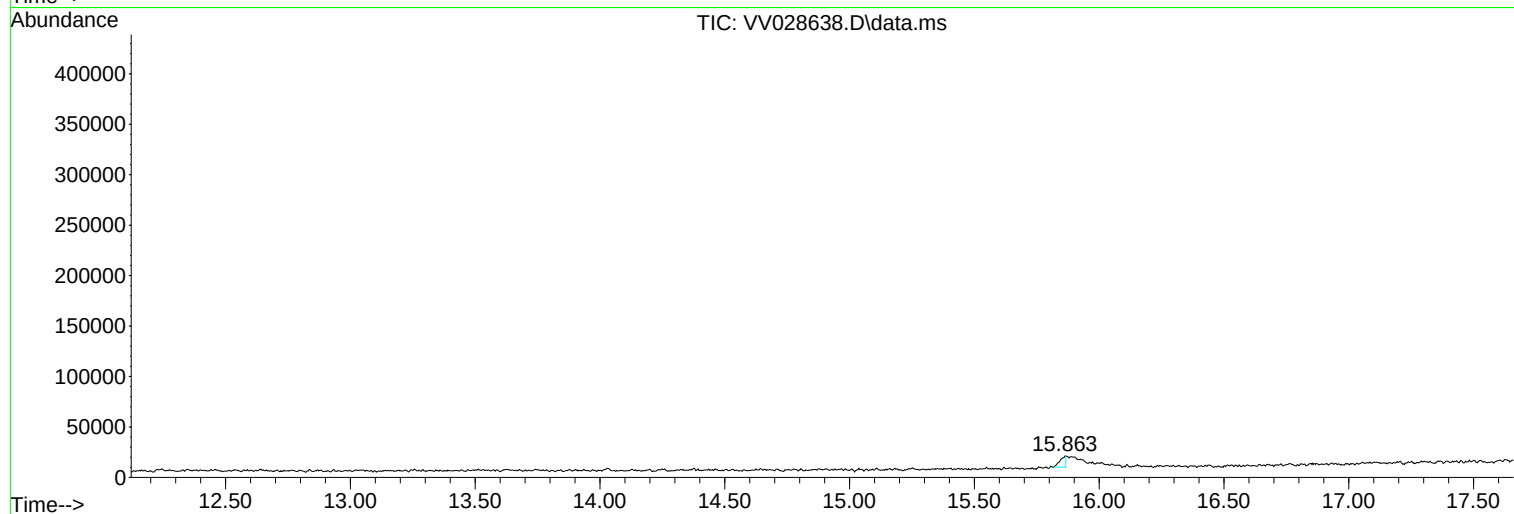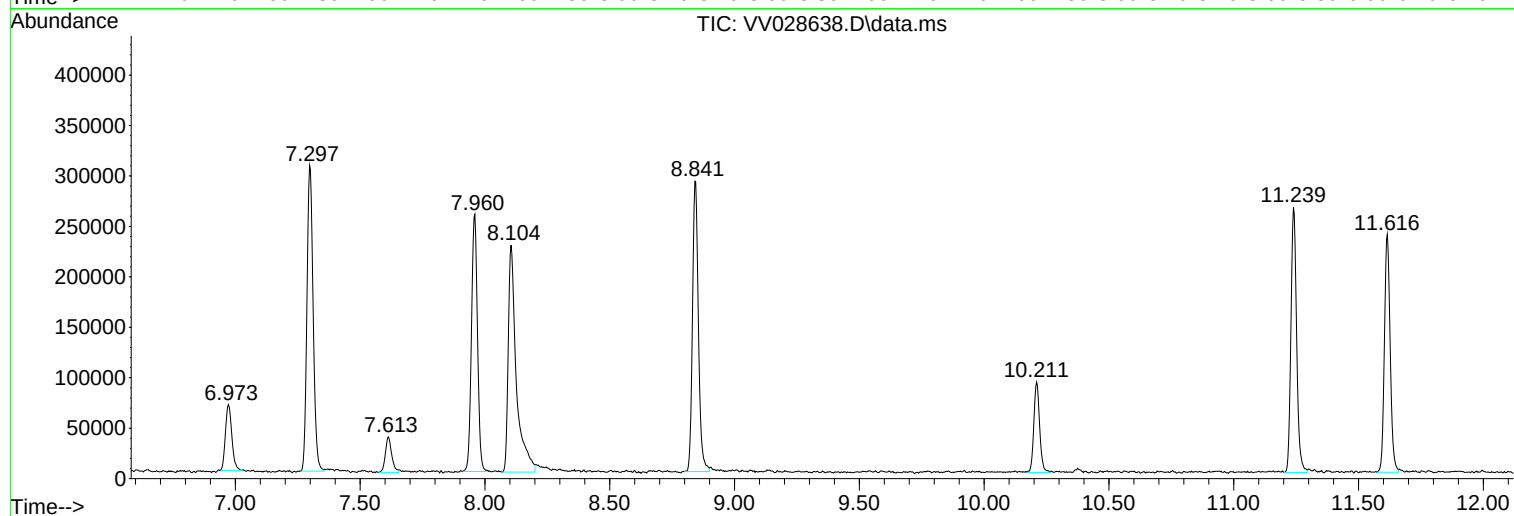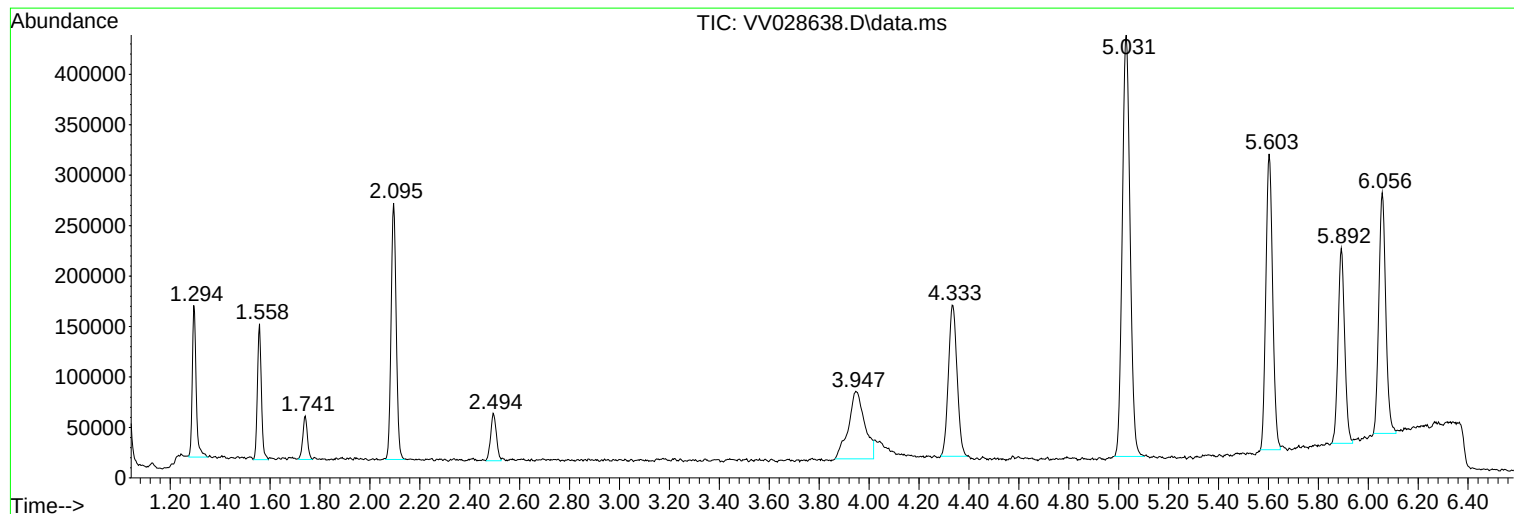

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028638.D
Acq On : 20 Oct 2022 16:32
Operator : SY/MD
Sample : N5173-05DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXTODL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028638.D
Acq On : 20 Oct 2022 16:32
Operator : SY/MD
Sample : N5173-05DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXTODL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
