

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
 Data File : VV028639.D
 Acq On : 20 Oct 2022 16:56
 Operator : SY/MD
 Sample : N5163-03DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BD713DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.230	49	59	63	rBV3	10110	16598	1.70%	0.276%
2	1.301	74	81	92	rBV	145757	150255	15.43%	2.500%
3	1.574	159	166	178	rVB	126228	143809	14.77%	2.393%
4	2.117	325	335	349	rBV	264115	379694	38.99%	6.317%
5	2.513	451	458	470	rVB	37249	59083	6.07%	0.983%
6	4.355	1018	1031	1047	rVB2	166138	386892	39.73%	6.437%
7	5.043	1232	1245	1264	rVB2	458942	973830	100.00%	16.201%
8	5.625	1411	1426	1449	rBV	199947	405377	41.63%	6.744%
9	6.082	1551	1568	1587	rBV	162597	337308	34.64%	5.612%
10	7.002	1843	1854	1871	rBV	65419	117213	12.04%	1.950%
11	7.326	1942	1955	1974	rBV	311006	546309	56.10%	9.089%
12	7.635	2043	2051	2071	rBV	32365	60111	6.17%	1.000%
13	7.979	2146	2158	2174	rVB	249668	415884	42.71%	6.919%
14	8.111	2186	2199	2229	rBV2	220120	508481	52.21%	8.459%
15	8.854	2417	2430	2456	rBV	302768	504041	51.76%	8.386%
16	10.214	2839	2853	2869	rBV	91006	150479	15.45%	2.503%
17	11.243	3163	3173	3190	rBV	271148	426844	43.83%	7.101%
18	11.619	3278	3290	3309	rBV	236928	388337	39.88%	6.461%
19	15.873	4594	4613	4616	rBV	13905	40273	4.14%	0.670%




Sum of corrected areas: 6010818

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028639.D
Acq On : 20 Oct 2022 16:56
Operator : SY/MD
Sample : N5163-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD713DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

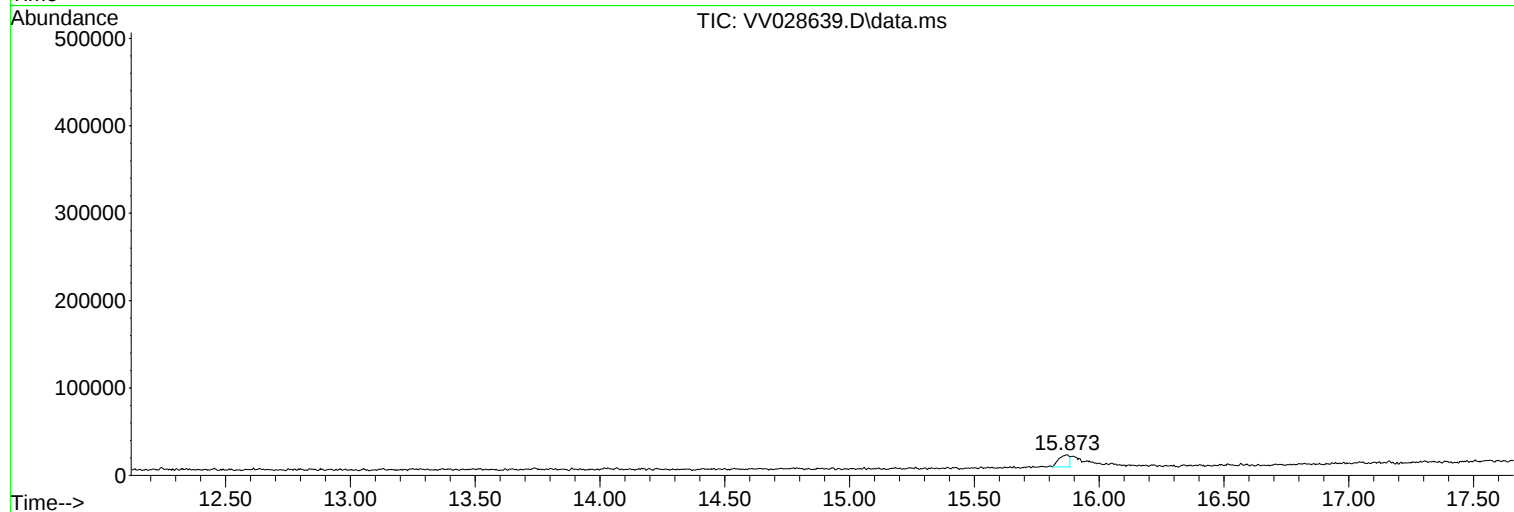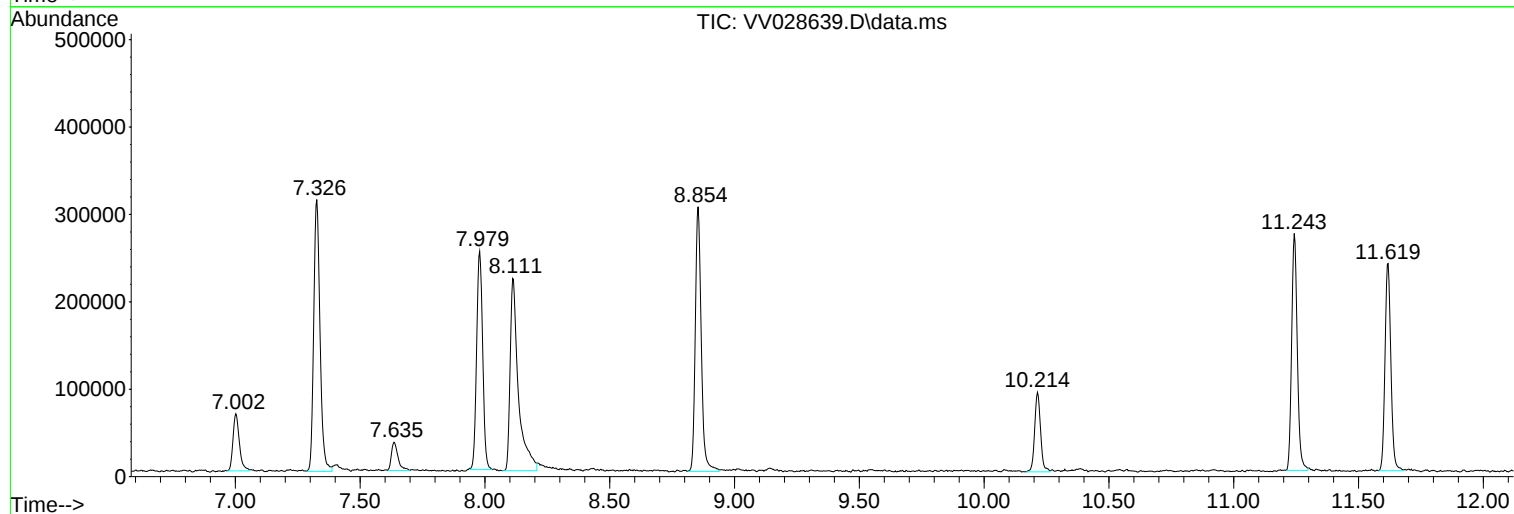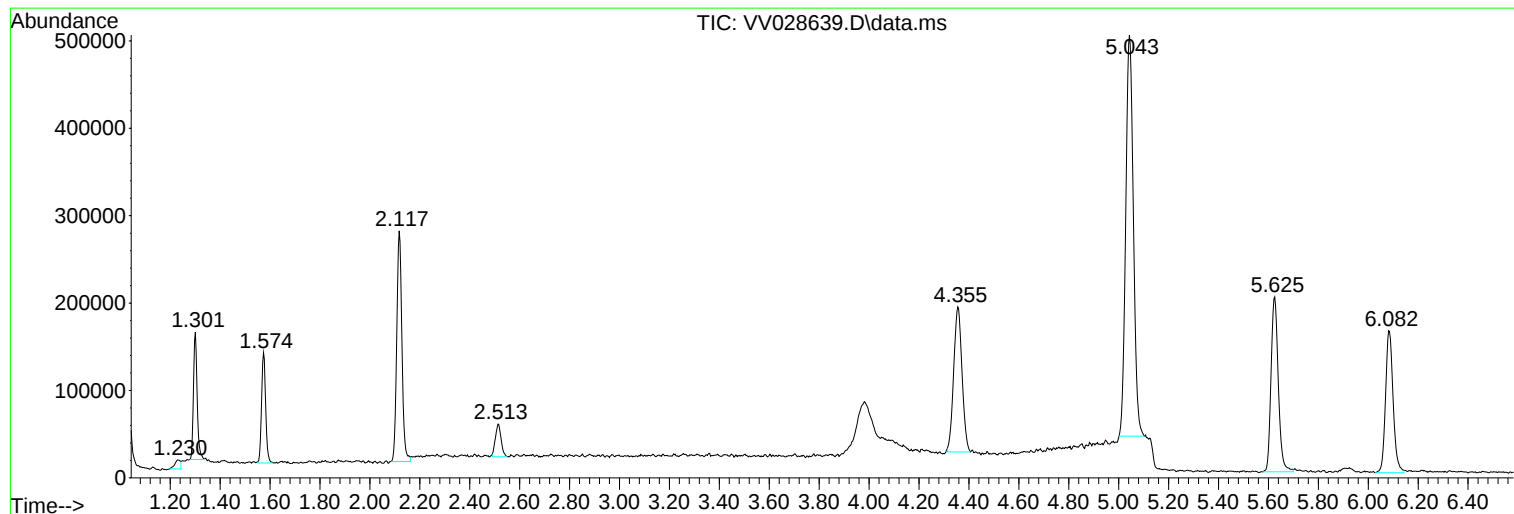

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028639.D
Acq On : 20 Oct 2022 16:56
Operator : SY/MD
Sample : N5163-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD713DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028639.D
Acq On : 20 Oct 2022 16:56
Operator : SY/MD
Sample : N5163-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD713DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------