

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
 Data File : VV028640.D
 Acq On : 20 Oct 2022 17:21
 Operator : SY/MD
 Sample : N5163-04DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BD714DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	73	79	96	rVB	145809	154474	17.33%	2.445%
2	1.558	154	161	175	rVB	123581	138499	15.53%	2.192%
3	2.095	319	328	343	rVB	245082	344962	38.69%	5.459%
4	2.494	444	452	464	rVB2	40737	67378	7.56%	1.066%
5	3.950	885	905	925	rBV	65479	267457	30.00%	4.233%
6	4.336	1012	1025	1044	rVB	147577	363035	40.72%	5.745%
7	5.031	1227	1241	1263	rVB2	407459	891551	100.00%	14.109%
8	5.603	1407	1419	1435	rBV2	297179	573119	64.28%	9.070%
9	6.056	1549	1560	1574	rBV	233921	446700	50.10%	7.069%
10	6.976	1835	1846	1860	rBV2	64770	117086	13.13%	1.853%
11	7.301	1936	1947	1966	rBV	303609	516146	57.89%	8.168%
12	7.613	2034	2044	2062	rVB3	34889	62711	7.03%	0.992%
13	7.960	2138	2152	2170	rBV	271793	455270	51.06%	7.205%
14	8.104	2187	2197	2231	rBV2	221082	497180	55.77%	7.868%
15	8.844	2415	2427	2443	rBV	296656	476098	53.40%	7.534%
16	10.211	2840	2852	2865	rBV	88898	144625	16.22%	2.289%
17	11.239	3157	3172	3193	rBV	265339	423381	47.49%	6.700%
18	11.616	3273	3289	3306	rBV	234387	379300	42.54%	6.003%




Sum of corrected areas: 6318972

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028640.D
Acq On : 20 Oct 2022 17:21
Operator : SY/MD
Sample : N5163-04DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD714DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

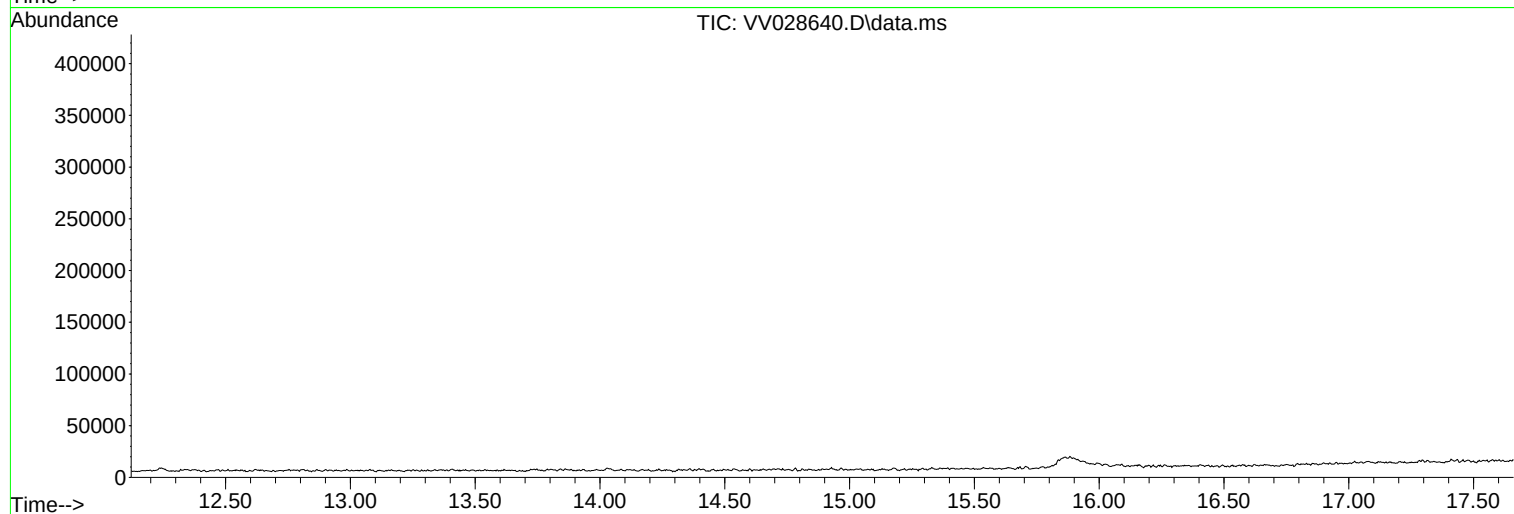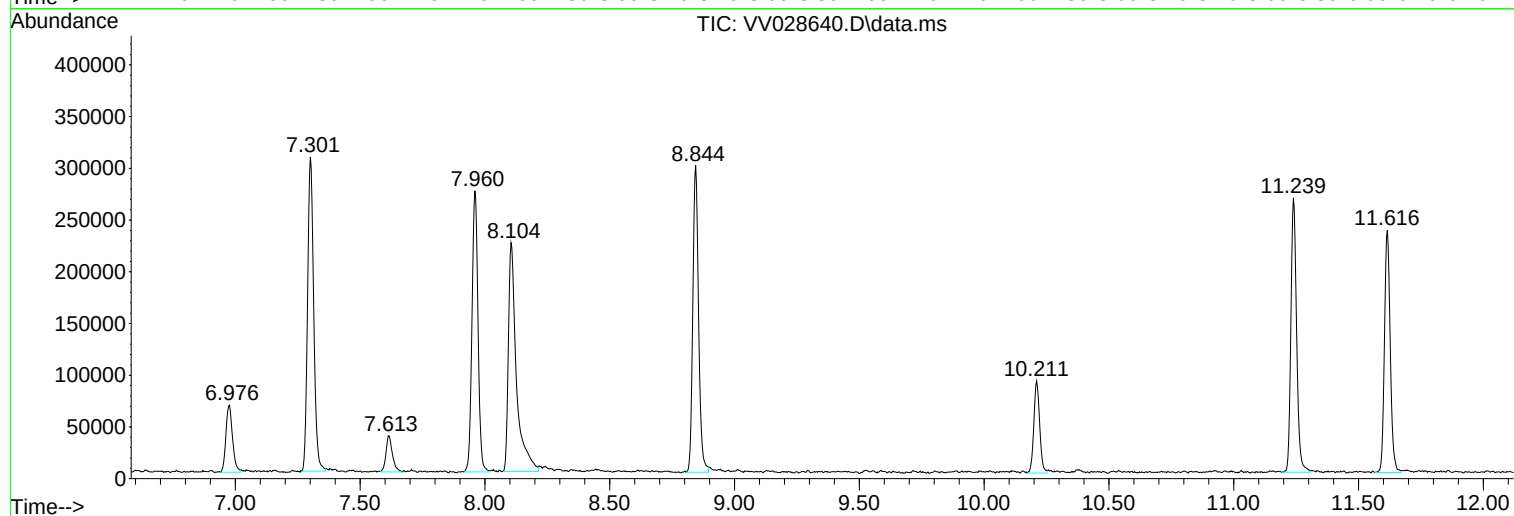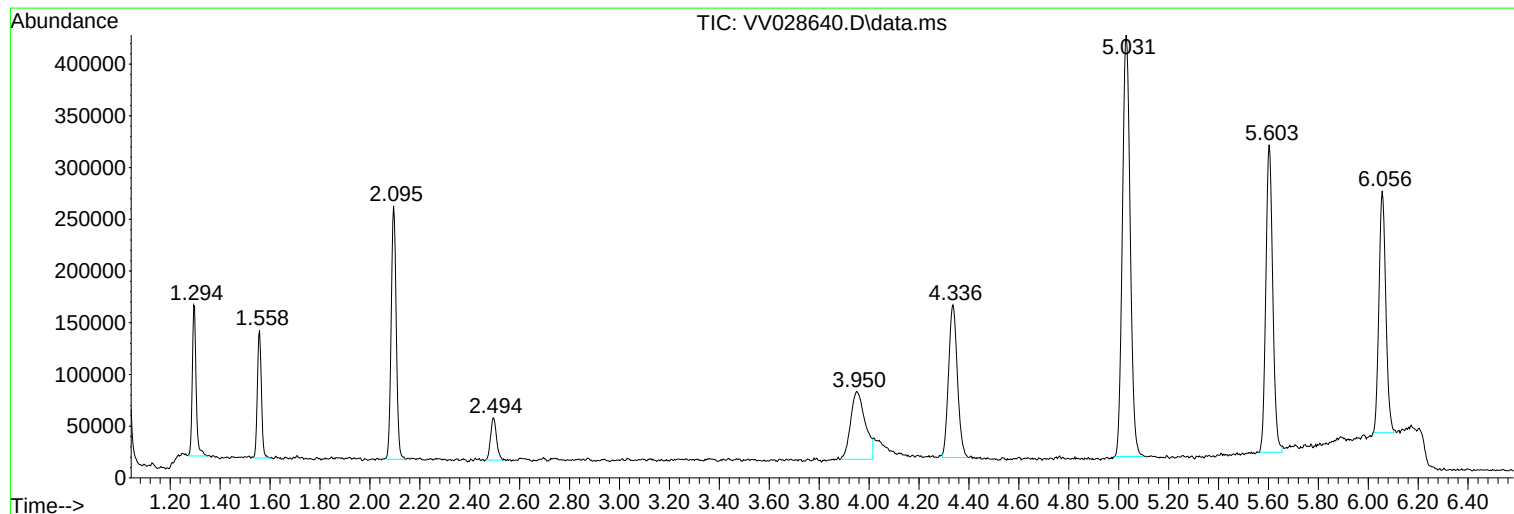

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028640.D
Acq On : 20 Oct 2022 17:21
Operator : SY/MD
Sample : N5163-04DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD714DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028640.D
Acq On : 20 Oct 2022 17:21
Operator : SY/MD
Sample : N5163-04DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD714DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc