

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
 Data File : VV028641.D
 Acq On : 20 Oct 2022 17:45
 Operator : SY/MD
 Sample : N5216-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA57

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.227	46	58	59	rBV10	12241	16734	1.84%	0.278%
2	1.294	73	79	94	rVB	144625	147921	16.30%	2.455%
3	1.555	153	160	174	rVB	117943	135767	14.96%	2.253%
4	2.095	314	328	340	rBV	235396	337822	37.23%	5.606%
5	2.770	526	538	554	rVB	95308	199699	22.01%	3.314%
6	3.957	889	907	927	rBV2	61102	250250	27.58%	4.153%
7	4.342	1011	1027	1048	rVB3	152992	443784	48.91%	7.365%
8	5.027	1227	1240	1260	rBV2	420773	907307	100.00%	15.057%
9	5.590	1405	1415	1432	rVB	334762	625341	68.92%	10.378%
10	6.050	1545	1558	1574	rBV2	149792	299998	33.06%	4.979%
11	6.976	1833	1846	1864	rBV	60046	111267	12.26%	1.847%
12	7.310	1936	1950	1968	rBV	264003	486895	53.66%	8.080%
13	7.628	2038	2049	2058	rBV	32117	54849	6.05%	0.910%
14	7.976	2147	2157	2169	rVB9	10027	18197	2.01%	0.302%
15	8.111	2187	2199	2230	rBV2	221775	501738	55.30%	8.327%
16	8.850	2414	2429	2444	rBV	299940	491227	54.14%	8.152%
17	10.214	2842	2853	2868	rVB	87631	139745	15.40%	2.319%
18	11.242	3159	3173	3191	rBV	281959	443991	48.94%	7.368%
19	11.615	3278	3289	3304	rBV	232337	375023	41.33%	6.224%
20	15.847	4589	4605	4609	rBV	17608	38206	4.21%	0.634%




Sum of corrected areas: 6025761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028641.D
Acq On : 20 Oct 2022 17:45
Operator : SY/MD
Sample : N5216-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

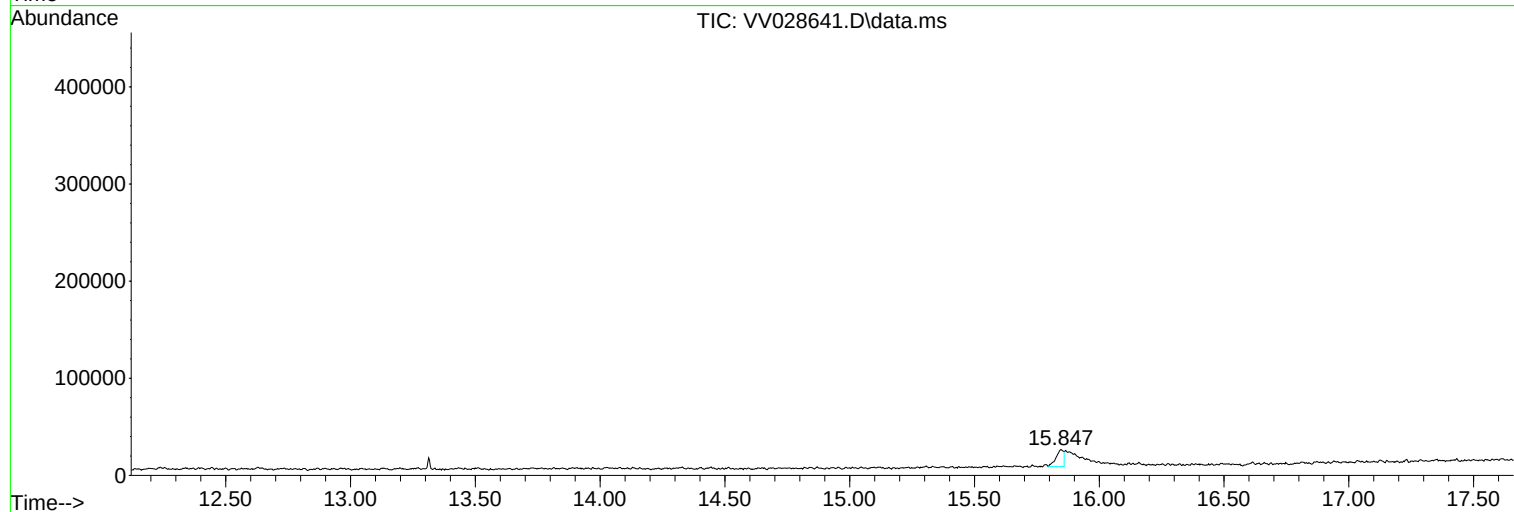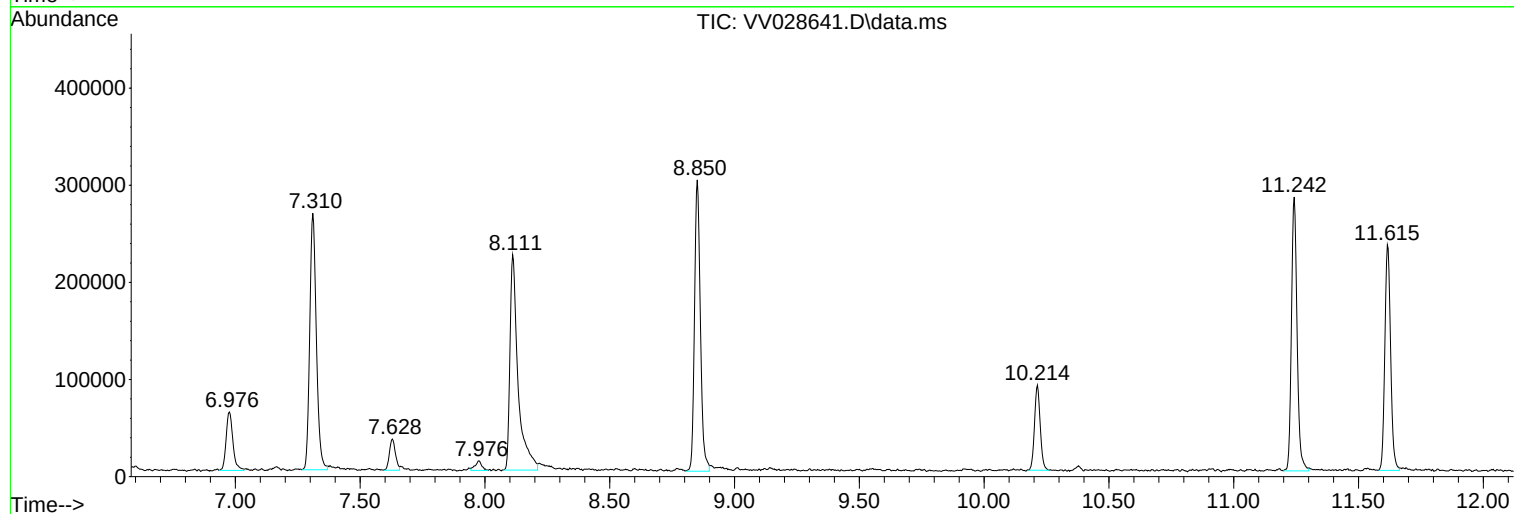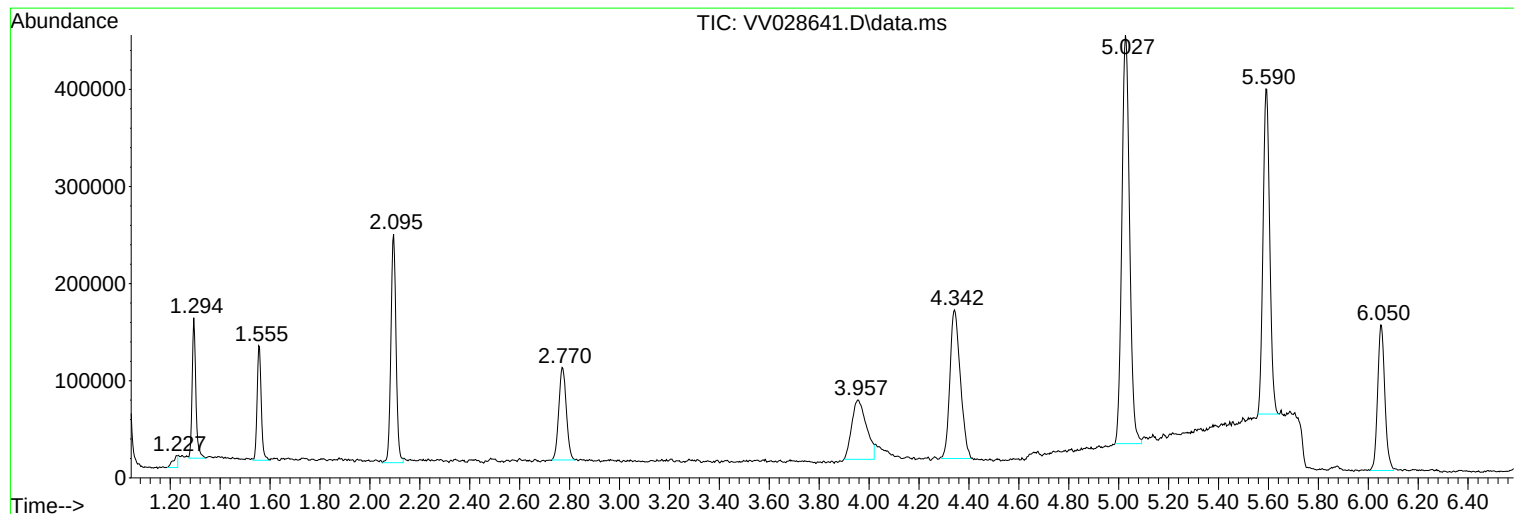

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028641.D
Acq On : 20 Oct 2022 17:45
Operator : SY/MD
Sample : N5216-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102022\
Data File : VV028641.D
Acq On : 20 Oct 2022 17:45
Operator : SY/MD
Sample : N5216-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc