

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032543.D
 Acq On : 20 Oct 2023 23:30
 Operator : SY/MD
 Sample : 04993-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 23 02:57:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 21 02:44:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	80915	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	92556	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	41392	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	24302	3.693	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.800%
7) Chloroethane-d5	1.532	69	23813	4.458	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.200%
11) 1,1-Dichloroethene-d2	2.060	65	10129	3.650	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.000%
20) 2-Butanone-d5	3.809	46	82786	49.730	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.460%
24) Chloroform-d	4.252	84	48780	4.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
26) 1,2-Dichloroethane-d4	4.947	65	27663	5.031	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.600%
32) Benzene-d6	4.963	84	92127	3.383	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	67.600%#
36) 1,2-Dichloropropane-d6	5.992	67	31519	3.493	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	69.800%
41) Toluene-d8	7.249	98	75363	3.026	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	60.600%#
43) trans-1,3-Dichloroprop...	7.561	79	10129	3.168	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	63.400%
46) 2-Hexanone-d5	8.030	63	62972	41.858	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.720%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	28682	4.545	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.800%
66) 1,2-Dichlorobenzene-d4	11.564	152	30527	3.974	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	79.400%#
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.188	75	5793	1.315	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032543.D
Acq On : 20 Oct 2023 23:30
Operator : SY/MD
Sample : 04993-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 23 02:57:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 21 02:44:24 2023
Response via : Initial Calibration

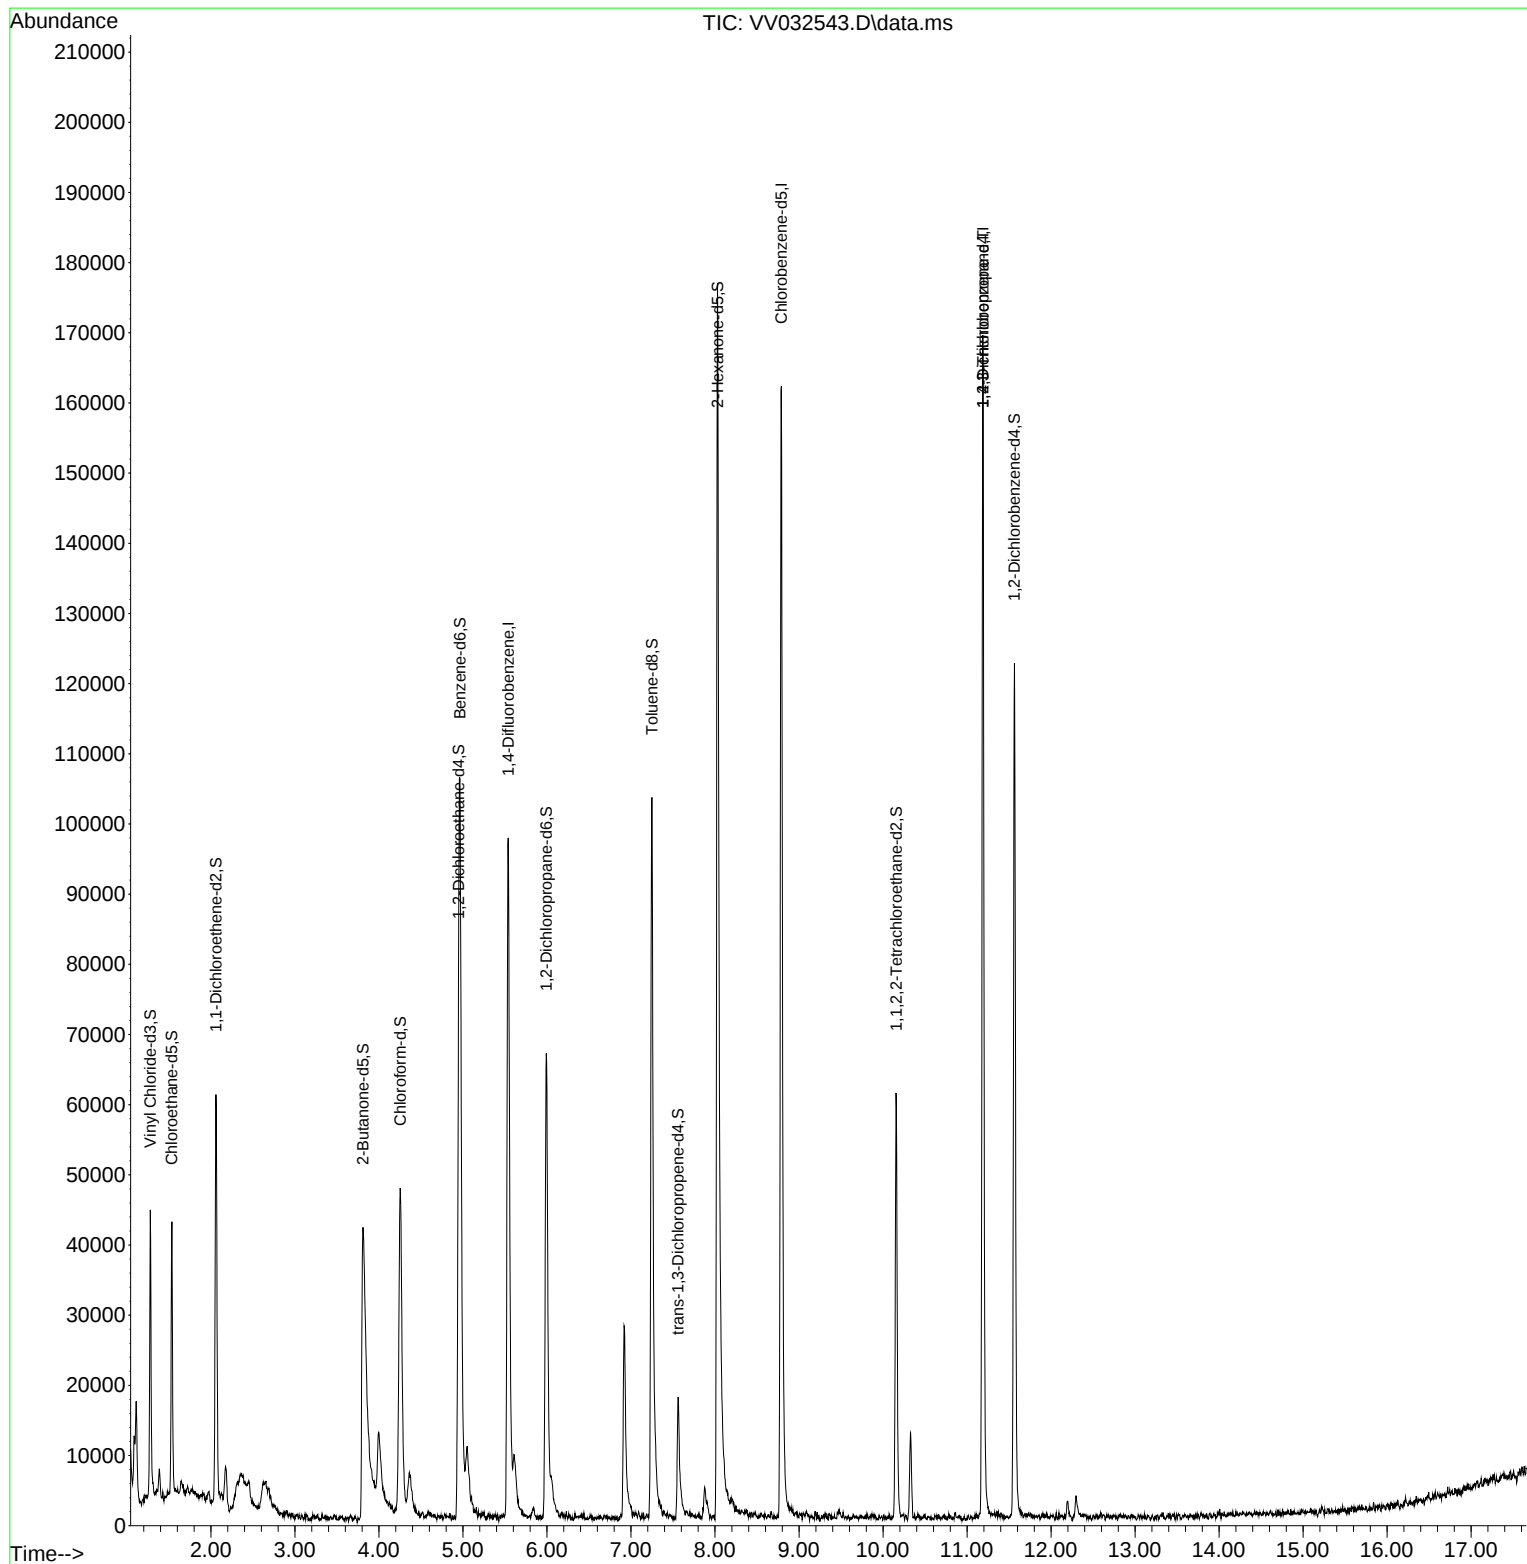

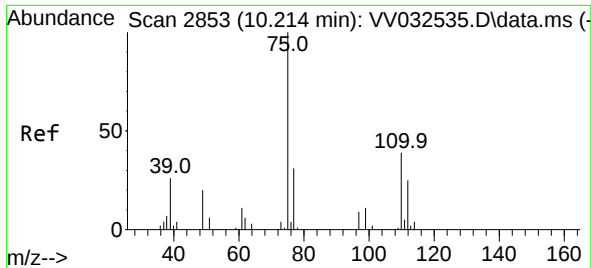

#61
1,2,3-Trichloropropane
Concen: 1.315 ug/L
RT: 11.188 min Scan# 31
Delta R.T. 0.974 min
Lab File: VV032543.D
Acq: 20 Oct 2023 23:30

Instrument :
MSVOA_V
ClientSampleId :

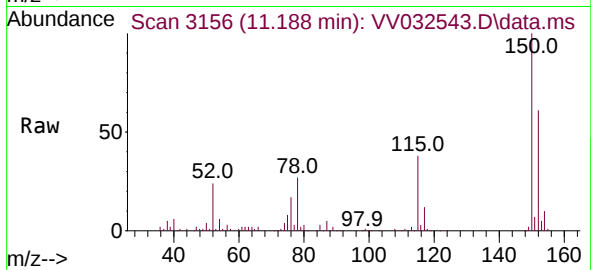

Tgt Ion	Ratio	Lower	Upper
75	100		
77	31.7	26.2	39.2
110	1.6	30.6	46.0

