




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032516.D
Acq On : 20 Oct 2023 11:52
Operator : SY/MD
Sample : 04903-11DL2 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF4DL2

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:05:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 20 23:03:10 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
Supervised By :Mahesh Dadoda 10/25/2023

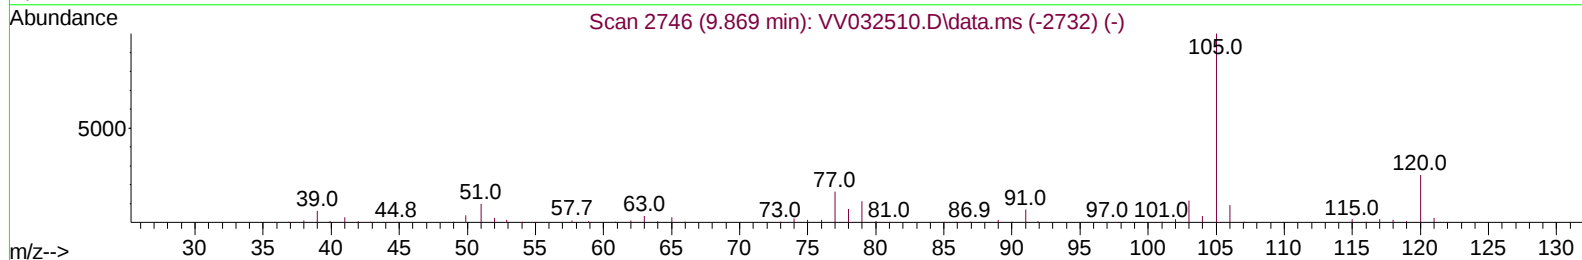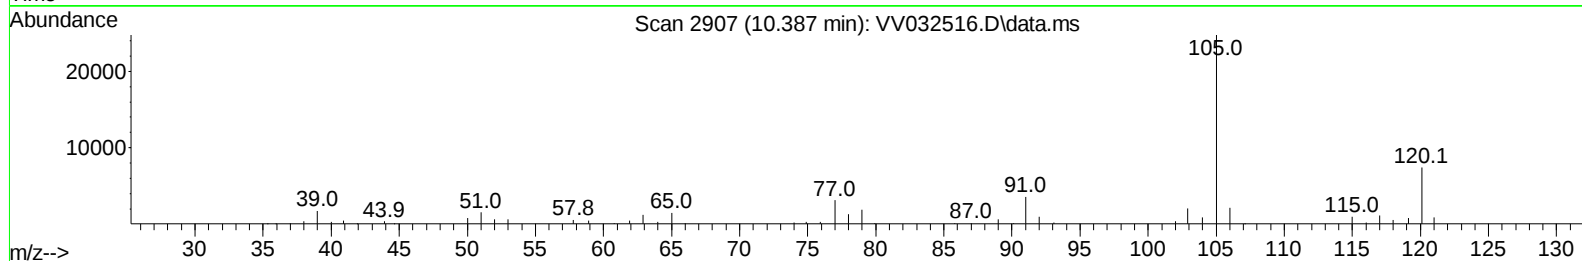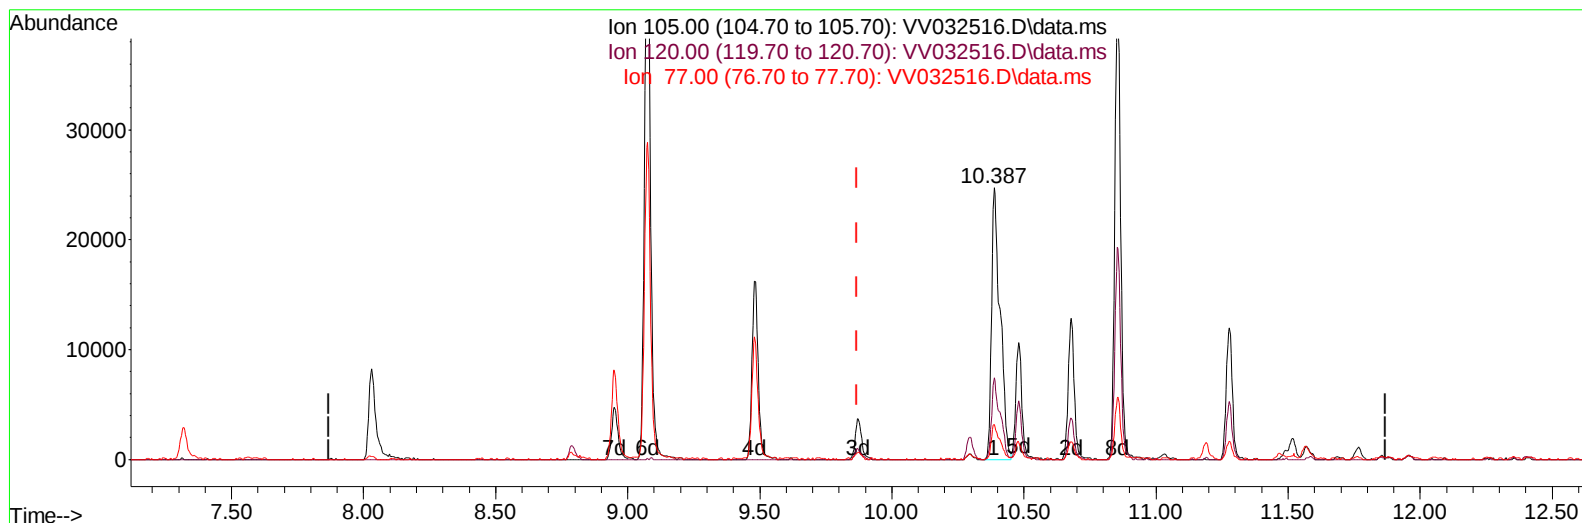

TIC: VV032516.D\data.ms

(60) Isopropylbenzene (T)

10.387min (+ 0.518) 1.35 ug/L

response 55263

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	26.30	30.05
77.00	15.80	13.03
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032516.D
 Acq On : 20 Oct 2023 11:52
 Operator : SY/MD
 Sample : 04903-11DL2 400X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF4DL2

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:05:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 20 23:03:10 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
 Supervised By :Mahesh Dadoda 10/25/2023

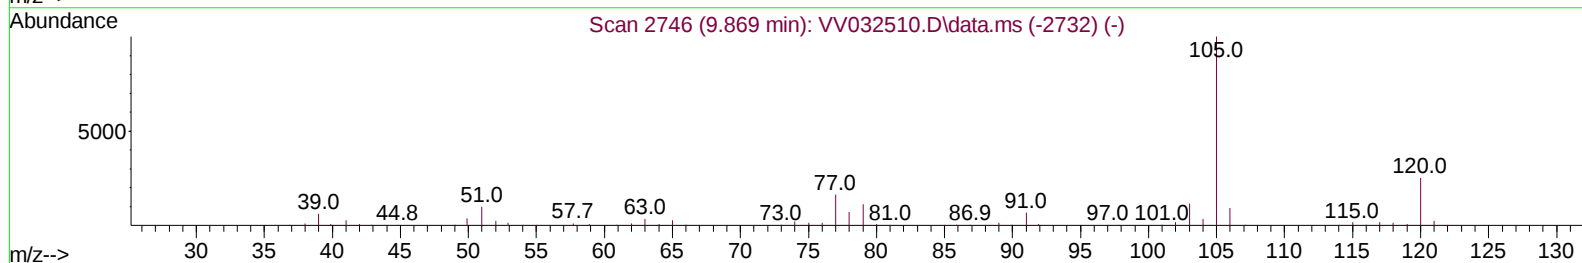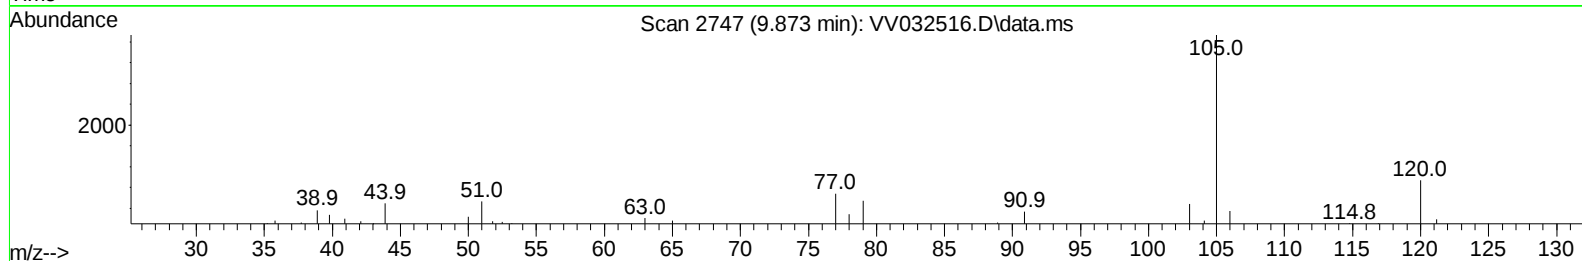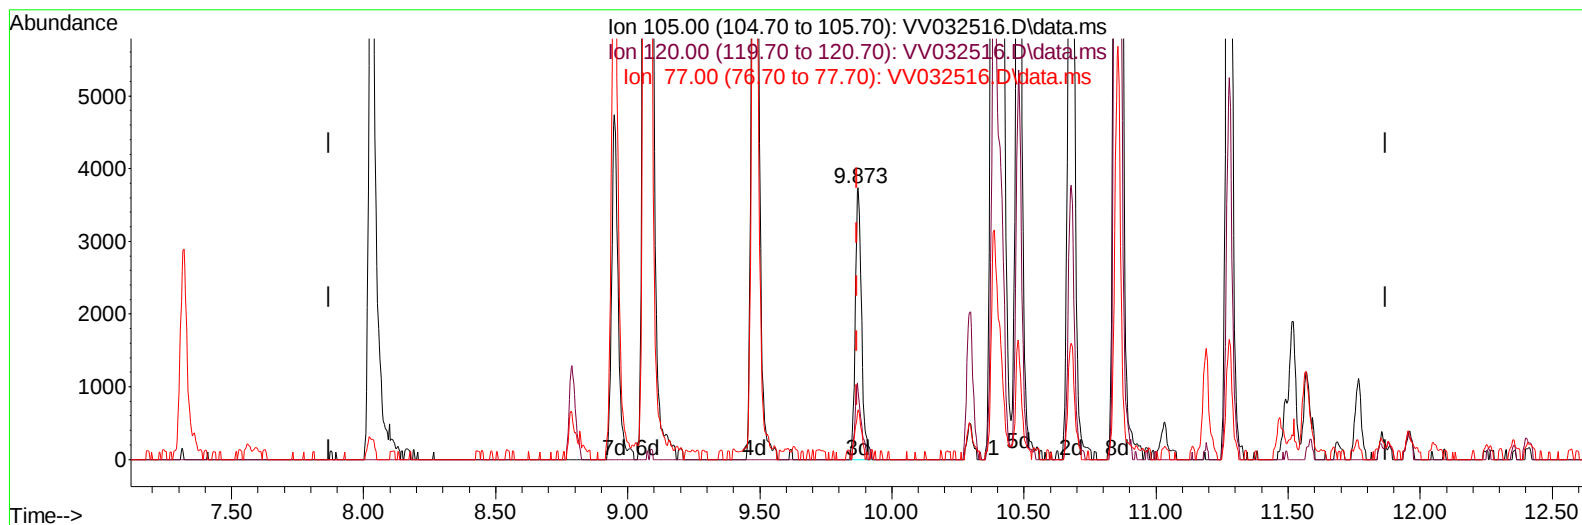

TIC: VV032516.D\data.ms

(60) Isopropylbenzene (T)

9.873min (+ 0.003) 0.15 ug/L m

response 6195

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	26.30	268.10#
77.00	15.80	116.22#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032516.D
 Acq On : 20 Oct 2023 11:52
 Operator : SY/MD
 Sample : 04903-11DL2 400X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF4DL2

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:05:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 20 23:03:10 2023
 Response via : Initial Calibration

Reviewed By : John Carlone 10/23/2023
 Supervised By : Mahesh Dadoda 10/25/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	91421	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	103978	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	52593	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	31303	4.210	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	84.200%	
7) Chloroethane-d5	1.532	69	29627	4.909	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	98.200%	
11) 1,1-Dichloroethene-d2	2.060	65	12556	4.004	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	80.000%	
20) 2-Butanone-d5	3.805	46	91996	48.912	ug/L	-0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	97.820%	
24) Chloroform-d	4.252	84	59411	4.530	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	90.600%	
26) 1,2-Dichloroethane-d4	4.947	65	31156	5.015	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	100.200%	
32) Benzene-d6	4.963	84	113520	3.710	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	74.200%	
36) 1,2-Dichloropropane-d6	5.992	67	41366	4.081	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	81.600%	
41) Toluene-d8	7.246	98	96239	3.440	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	68.800%#	
43) trans-1,3-Dichloroprop...	7.558	79	12737	3.546	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	71.000%	
46) 2-Hexanone-d5	8.030	63	74700	44.199	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	88.400%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	32934	4.645	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	92.800%	
66) 1,2-Dichlorobenzene-d4	11.564	152	39679	4.066	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	81.400%	
Target Compounds						
					Qvalue	
16) Methylene chloride	2.449	84	5690	0.651	ug/L	97
30) Cyclohexane	4.584	56	6843	0.440	ug/L #	92
35) Methylcyclohexane	6.053	83	2410	0.156	ug/L #	76
42) Toluene	7.317	91	437680	11.215	ug/L	100
52) Ethylbenzene	8.950	91	143835	3.310	ug/L	100
53) m,p-Xylene	9.075	106	167282	10.379	ug/L	98
54) o-Xylene	9.480	106	61204	3.941	ug/L	98
60) Isopropylbenzene	9.873	105	6195m	0.152	ug/L	
62) 1,3,5-Trimethylbenzene	10.480	105	16894	0.507	ug/L	99
63) 1,2,4-Trimethylbenzene	10.853	105	65174	1.965	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032516.D
Acq On : 20 Oct 2023 11:52
Operator : SY/MD
Sample : 04903-11DL2 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF4DL2

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:05:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 20 23:03:10 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
Supervised By :Mahesh Dadoda 10/25/2023

