




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032530.D
 Acq On : 20 Oct 2023 17:52
 Operator : SY/MD
 Sample : 04994-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B25

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:08:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 20 23:03:10 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
 Supervised By :Mahesh Dadoda 10/24/2023

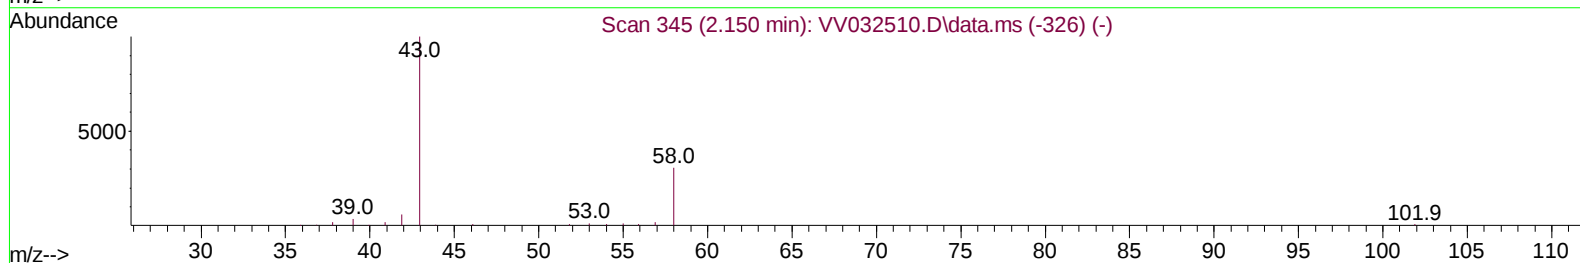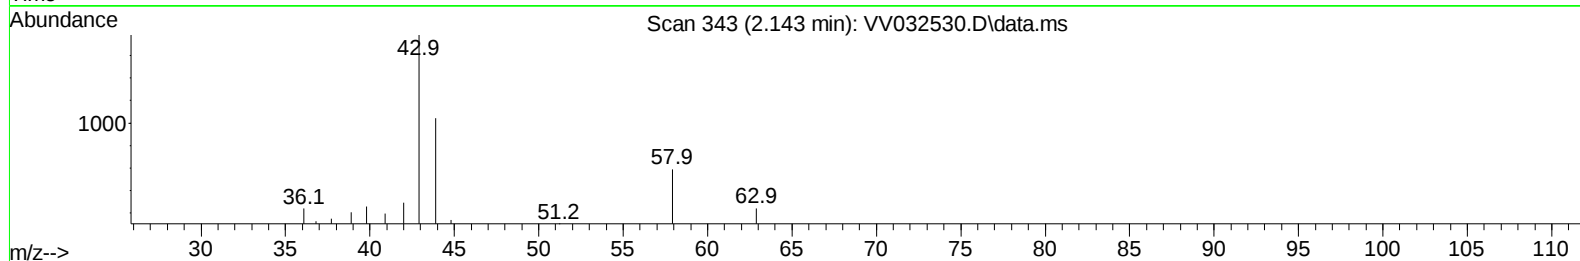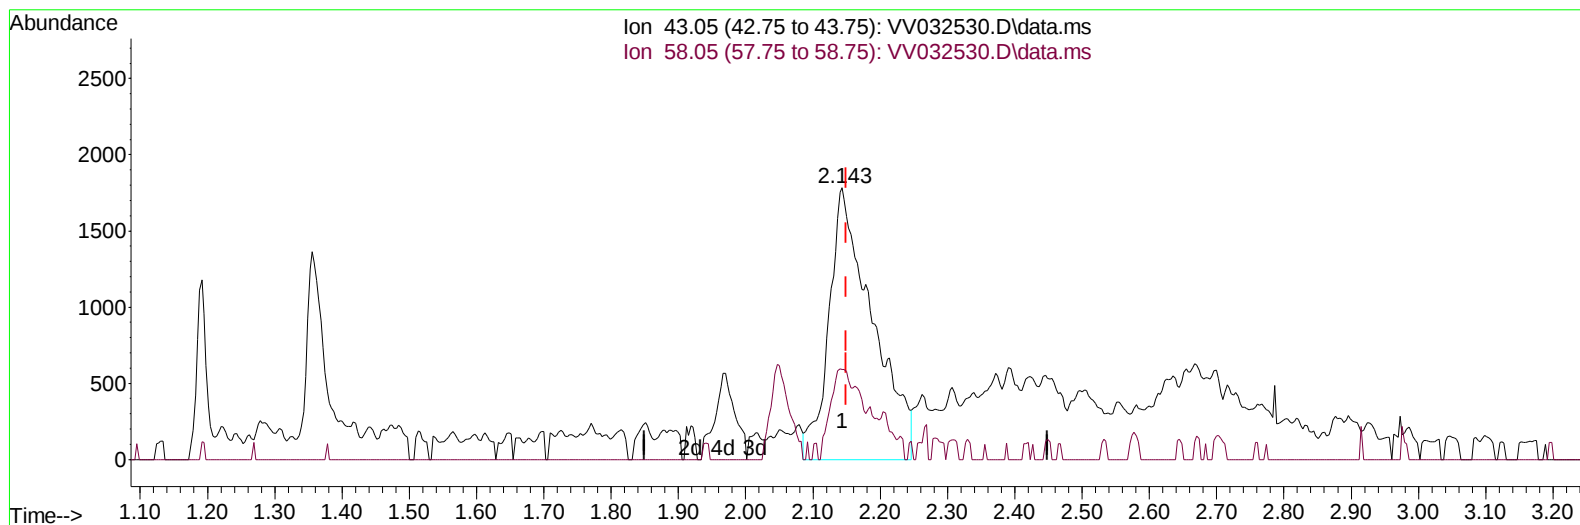

TIC: VV032530.D\data.ms

(13) Acetone (T)

2.143min (-0.006) 5.78 ug/L m

response 7980

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.00	16.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032530.D
 Acq On : 20 Oct 2023 17:52
 Operator : SY/MD
 Sample : 04994-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B25

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:08:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 20 23:03:10 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
 Supervised By :Mahesh Dadoda 10/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	87092	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	98637	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	45856	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	27414	3.870	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	77.400%		
7) Chloroethane-d5	1.532	69	26622	4.630	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	92.600%		
11) 1,1-Dichloroethene-d2	2.060	65	11164	3.737	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	74.800%		
20) 2-Butanone-d5	3.818	46	84462	47.138	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	94.280%		
24) Chloroform-d	4.256	84	57973	4.640	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	92.800%		
26) 1,2-Dichloroethane-d4	4.947	65	29584	4.998	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	100.000%		
32) Benzene-d6	4.963	84	101285	3.490	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	69.800%#		
36) 1,2-Dichloropropane-d6	5.989	67	34972	3.637	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	72.800%		
41) Toluene-d8	7.246	98	85142	3.208	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	64.200%#		
43) trans-1,3-Dichloroprop...	7.561	79	12301	3.610	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	72.200%		
46) 2-Hexanone-d5	8.031	63	66813	41.673	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	83.340%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	29752	4.423	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	88.400%		
66) 1,2-Dichlorobenzene-d4	11.564	152	33224	3.904	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	78.000%#		
Target Compounds						
13) Acetone	2.143	43	7980m	5.778	ug/L	
25) Chloroform	4.278	83	121477	8.996	ug/L	99
38) Bromodichloromethane	6.439	83	27901	2.528	ug/L	98
49) Dibromochloromethane	8.182	129	4994	0.732	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032530.D
Acq On : 20 Oct 2023 17:52
Operator : SY/MD
Sample : 04994-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B25

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:08:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 20 23:03:10 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
Supervised By :Mahesh Dadoda 10/24/2023

