




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032531.D
 Acq On : 20 Oct 2023 18:17
 Operator : SY/MD
 Sample : 04994-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B26

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:08:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 20 23:03:10 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
 Supervised By :Mahesh Dadoda 10/24/2023

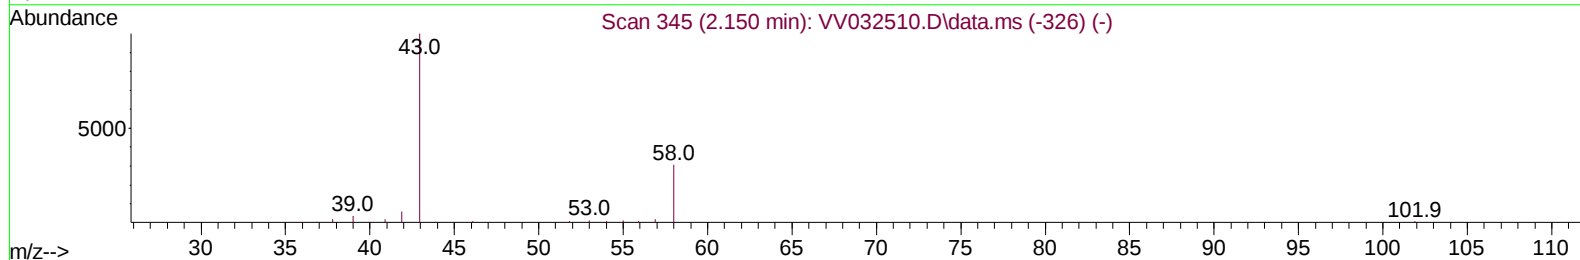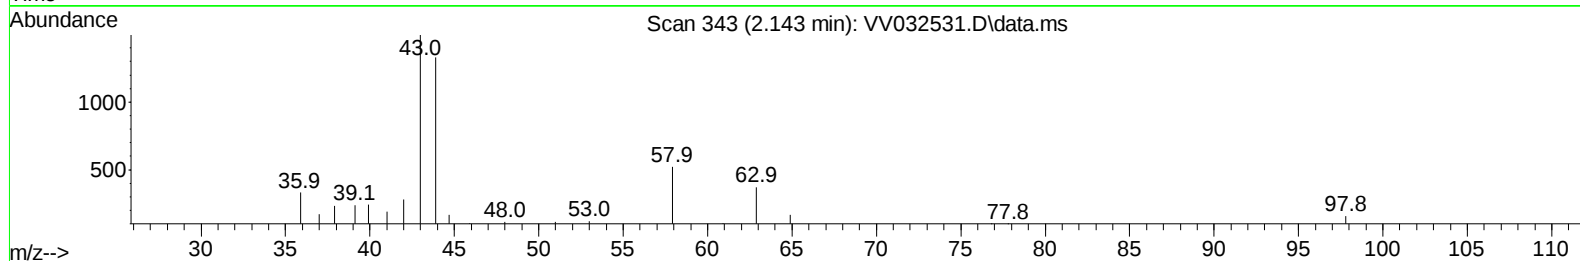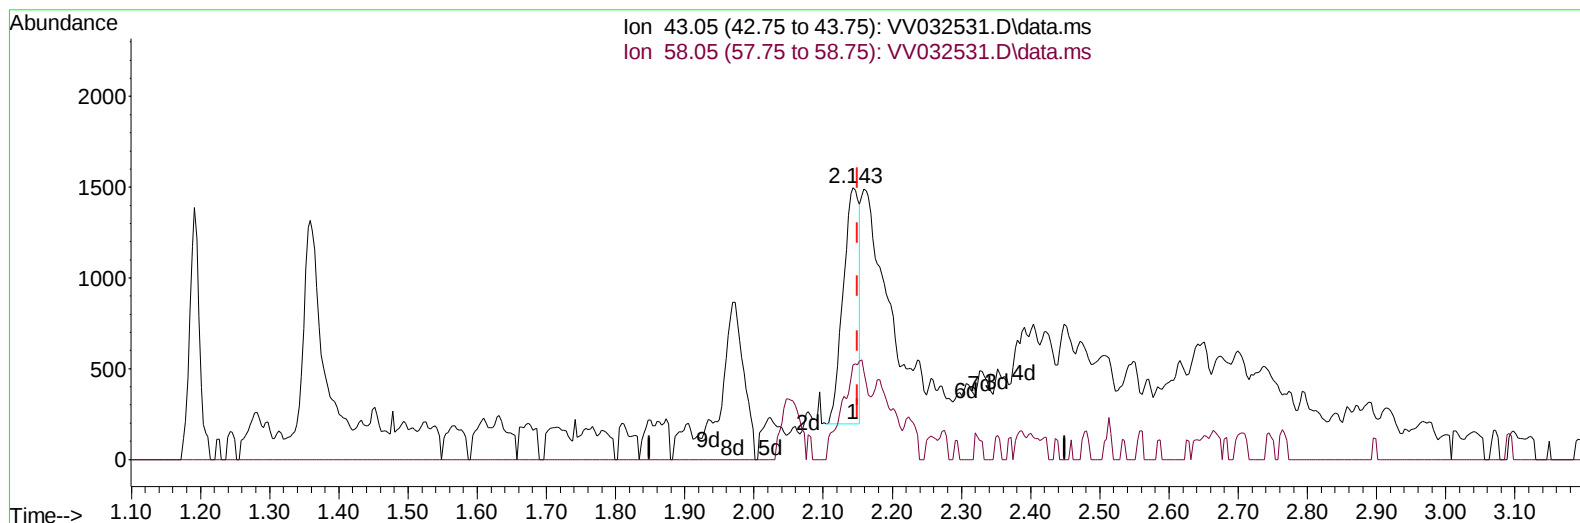

TIC: VV032531.D\data.ms

(13) Acetone (T)

2.143min (-0.006) 1.63 ug/L

response 2131

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.00	64.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032531.D
 Acq On : 20 Oct 2023 18:17
 Operator : SY/MD
 Sample : 04994-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B26

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:08:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 20 23:03:10 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
 Supervised By :Mahesh Dadoda 10/24/2023

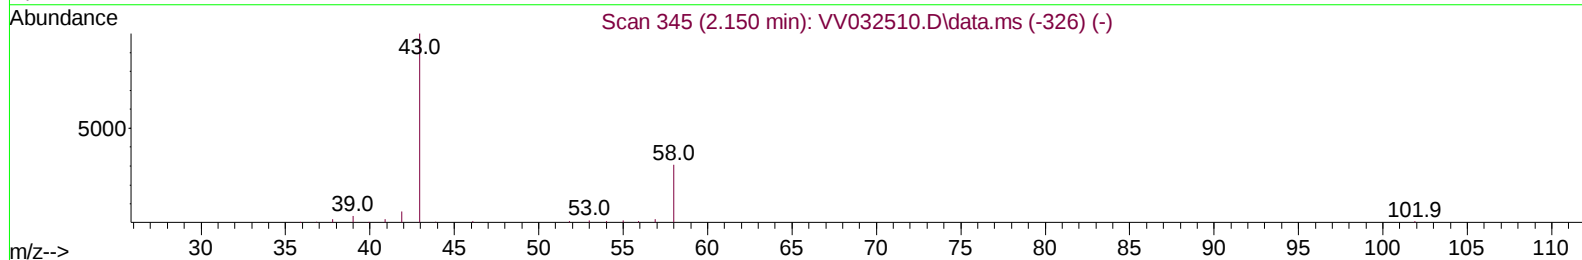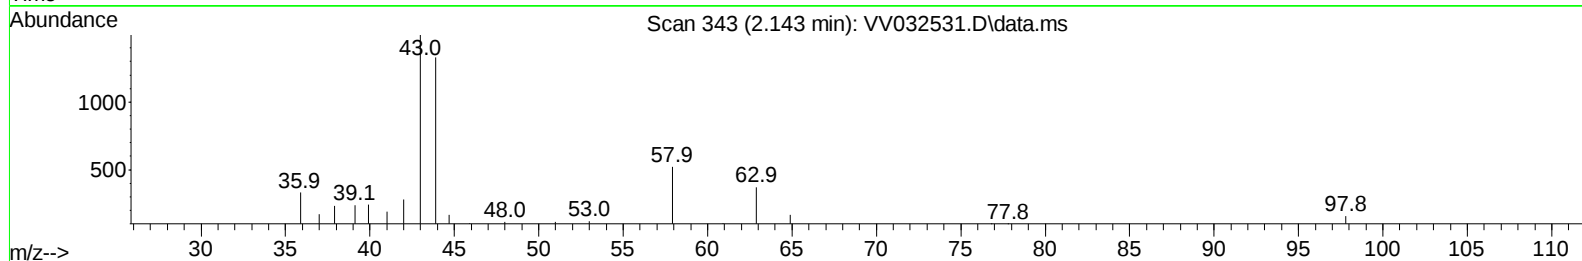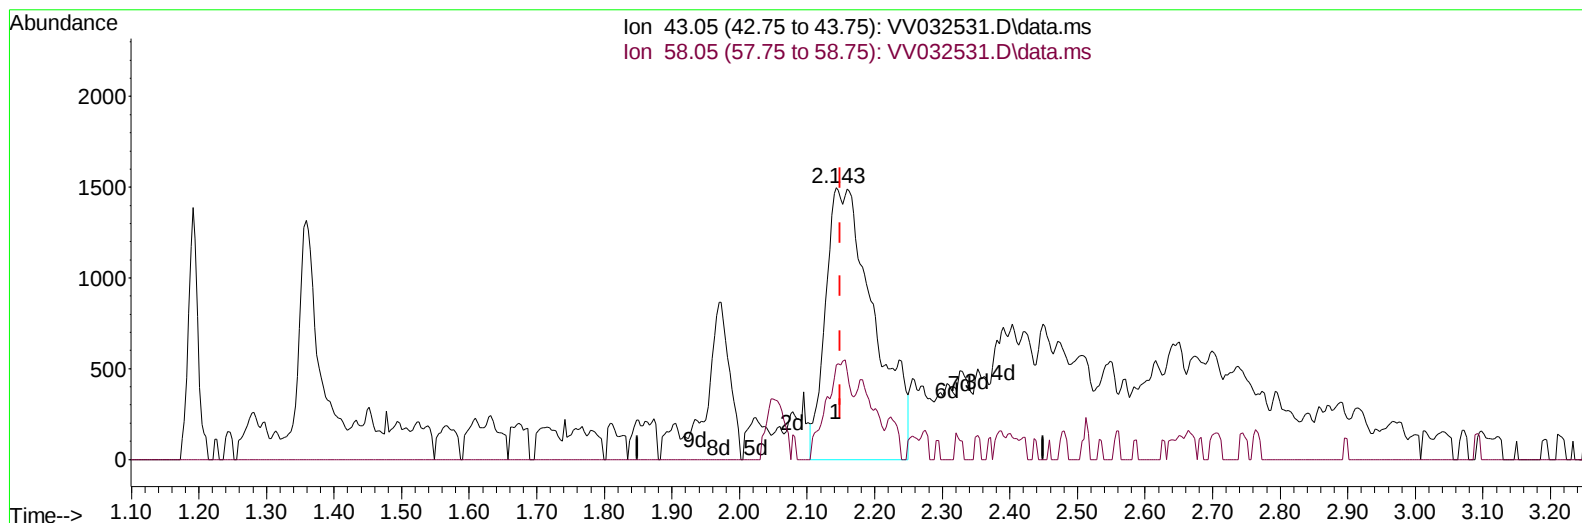

TIC: VV032531.D\data.ms

(13) Acetone (T)

2.143min (-0.006) 5.71 ug/L m

response 7450

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.00	18.38
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032531.D
Acq On : 20 Oct 2023 18:17
Operator : SY/MD
Sample : 04994-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B26

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:08:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 20 23:03:10 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
Supervised By :Mahesh Dadoda 10/24/2023

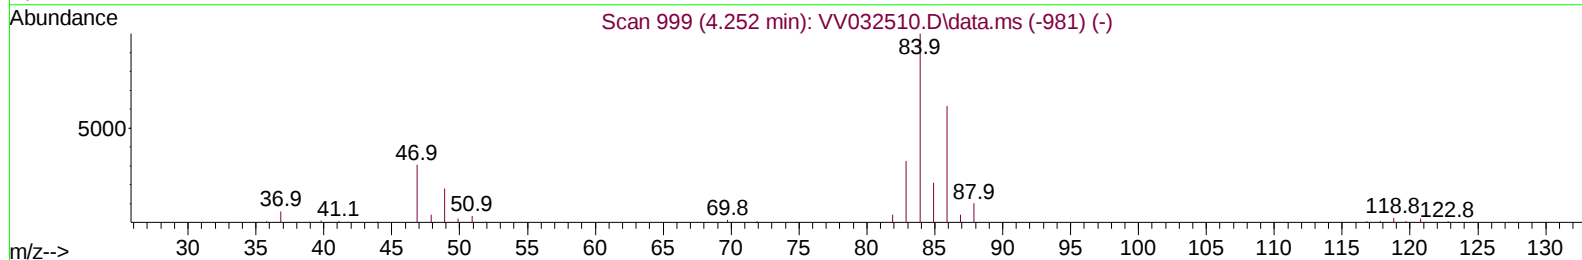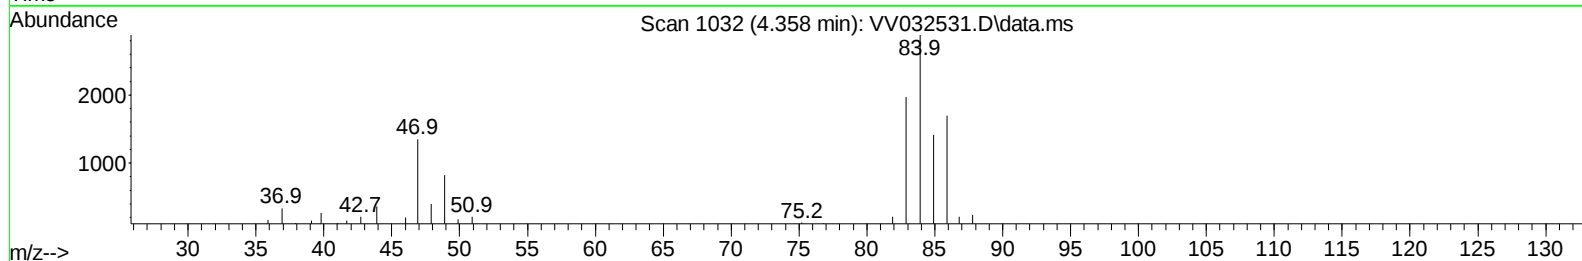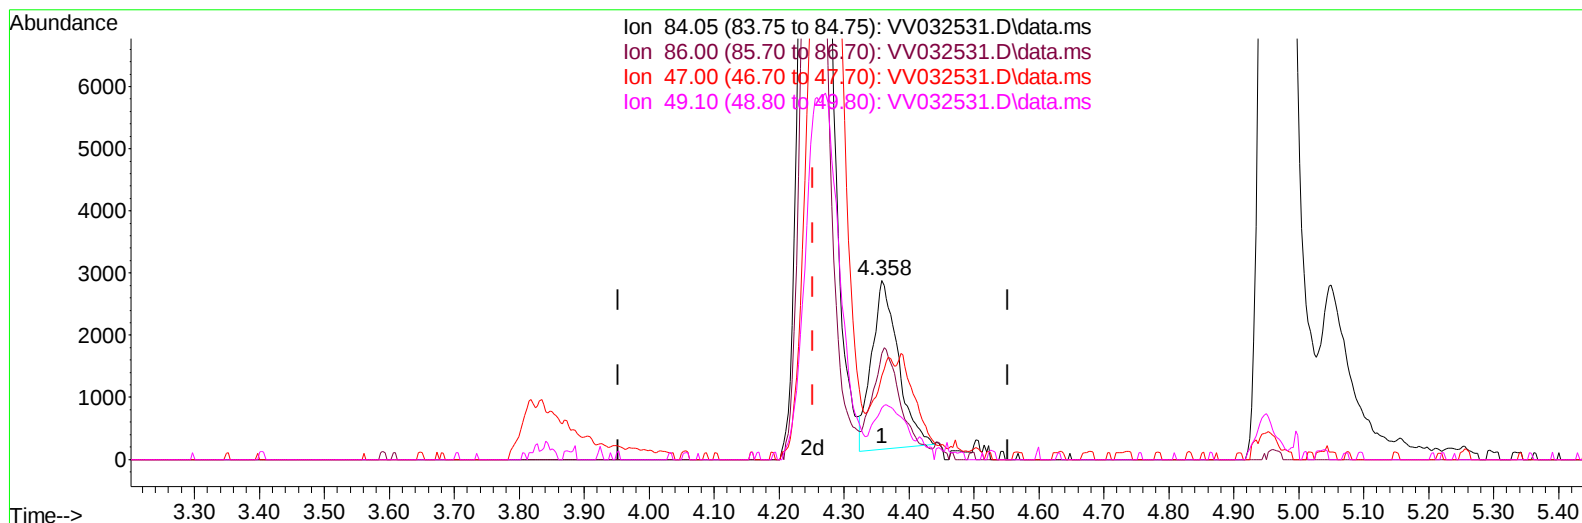

TIC: VV032531.D\data.ms

(24) Chloroform-d (S)

4.358min (+ 0.106) 0.65 ug/L

response 7730

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	61.90	62.45
47.00	43.10	38.73
49.10	25.00	26.66




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032531.D
Acq On : 20 Oct 2023 18:17
Operator : SY/MD
Sample : 04994-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B26

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:08:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 20 23:03:10 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
Supervised By :Mahesh Dadoda 10/24/2023

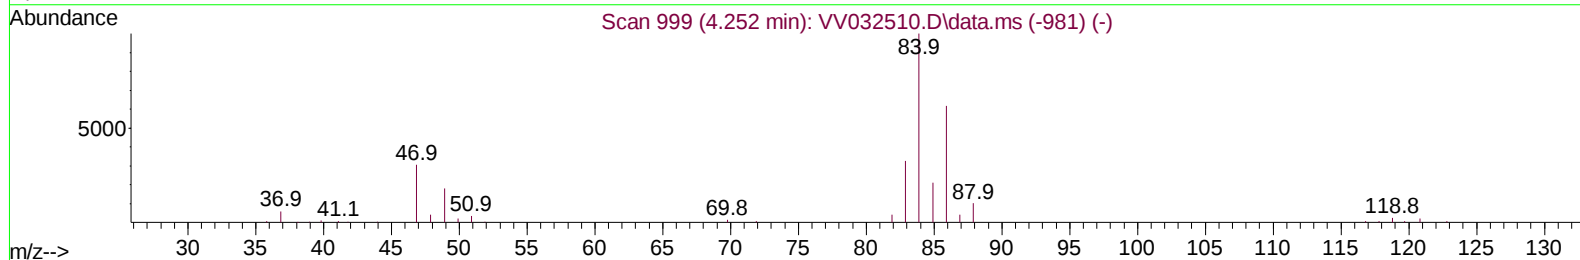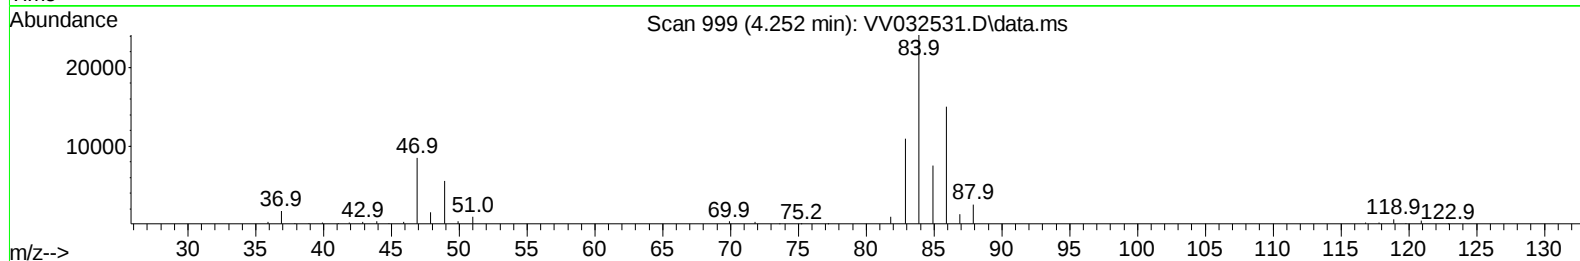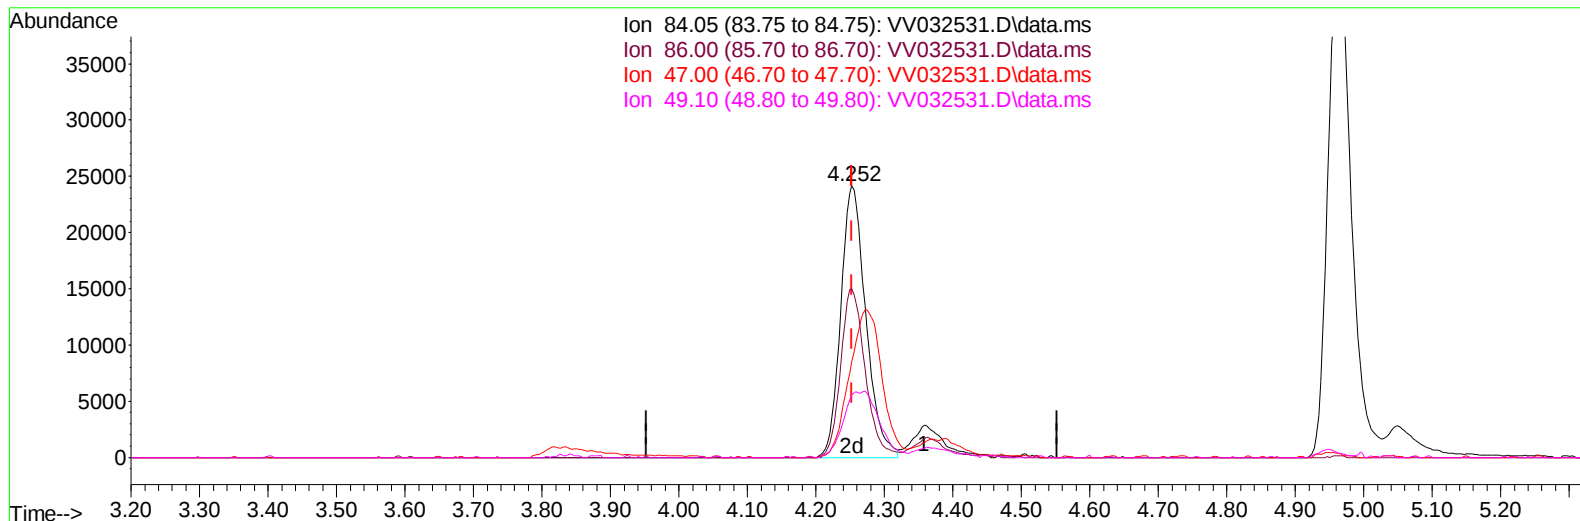

TIC: VV032531.D\data.ms

(24) Chloroform-d (S)

4.252min (0.000) 5.20 ug/L m

response 61346

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	61.90	7.87#
47.00	43.10	4.88#
49.10	25.00	3.36#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032531.D
 Acq On : 20 Oct 2023 18:17
 Operator : SY/MD
 Sample : 04994-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B26

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:08:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 20 23:03:10 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
 Supervised By :Mahesh Dadoda 10/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	82279	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	90150	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	41834	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	28474	4.255	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	85.200%		
7) Chloroethane-d5	1.532	69	27534	5.069	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	101.400%		
11) 1,1-Dichloroethene-d2	2.059	65	11725	4.155	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	83.000%		
20) 2-Butanone-d5	3.818	46	92092	54.403	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	108.800%		
24) Chloroform-d	4.252	84	61346m	5.197	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	104.000%		
26) 1,2-Dichloroethane-d4	4.947	65	29873	5.342	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	106.800%		
32) Benzene-d6	4.963	84	106199	4.004	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	80.000%		
36) 1,2-Dichloropropane-d6	5.992	67	39777	4.526	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	90.600%		
41) Toluene-d8	7.246	98	90138	3.716	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	74.400%		
43) trans-1,3-Dichloroprop...	7.561	79	12334	3.960	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	79.200%		
46) 2-Hexanone-d5	8.030	63	72129	49.224	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	98.440%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	32126	5.226	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	104.600%		
66) 1,2-Dichlorobenzene-d4	11.564	152	35206	4.535	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	90.800%		
Target Compounds						
						Qvalue
13) Acetone	2.143	43	7450m	5.710	ug/L	
25) Chloroform	4.278	83	117776	9.232	ug/L	97
38) Bromodichloromethane	6.439	83	27102	2.687	ug/L	99
49) Dibromochloromethane	8.178	129	4827	0.774	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032531.D
Acq On : 20 Oct 2023 18:17
Operator : SY/MD
Sample : 04994-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B26

Manual IntegrationsAPPROVED

Quant Time: Oct 20 23:08:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 20 23:03:10 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
Supervised By :Mahesh Dadoda 10/24/2023

