




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032556.D
Acq On : 21 Oct 2023 04:47
Operator : SY/MD
Sample : 04993-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Manual IntegrationsAPPROVED

Quant Time: Oct 23 03:01:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 21 02:44:24 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
Supervised By :Mahesh Dadoda 10/24/2023

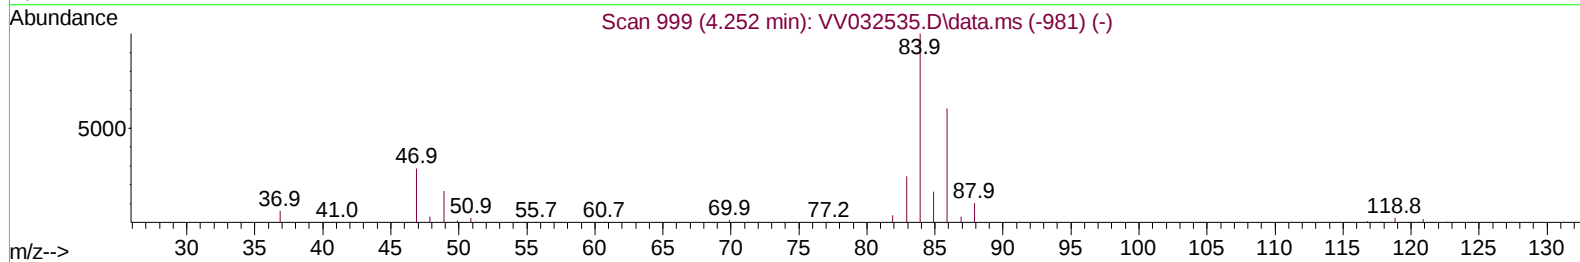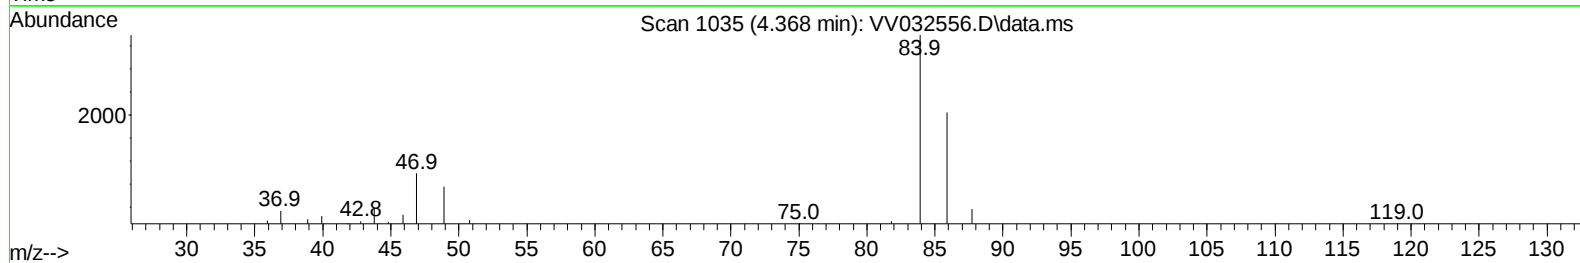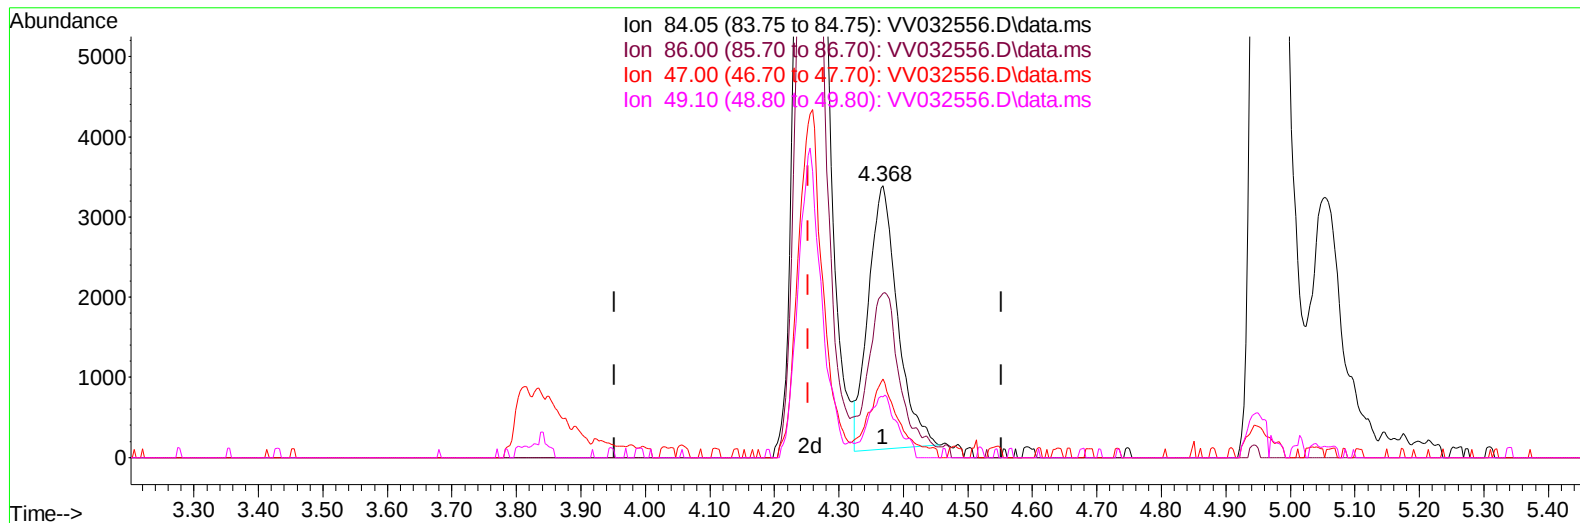

TIC: VV032556.D\data.ms

(24) Chloroform-d (S)

4.368min (+ 0.116) 0.98 ug/L

response 10338

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	61.90	60.00
47.00	43.10	31.87
49.10	25.00	23.53




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032556.D
Acq On : 21 Oct 2023 04:47
Operator : SY/MD
Sample : 04993-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAX0

Manual IntegrationsAPPROVED

Quant Time: Oct 23 03:01:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 21 02:44:24 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
Supervised By :Mahesh Dadoda 10/24/2023

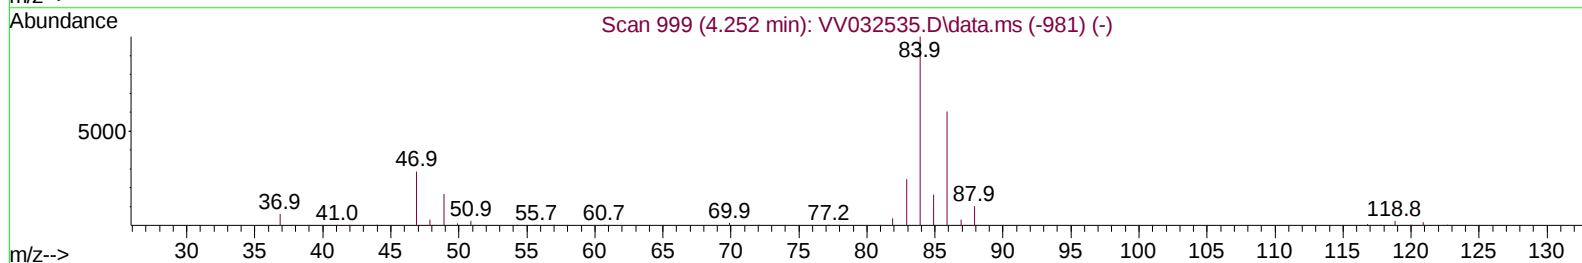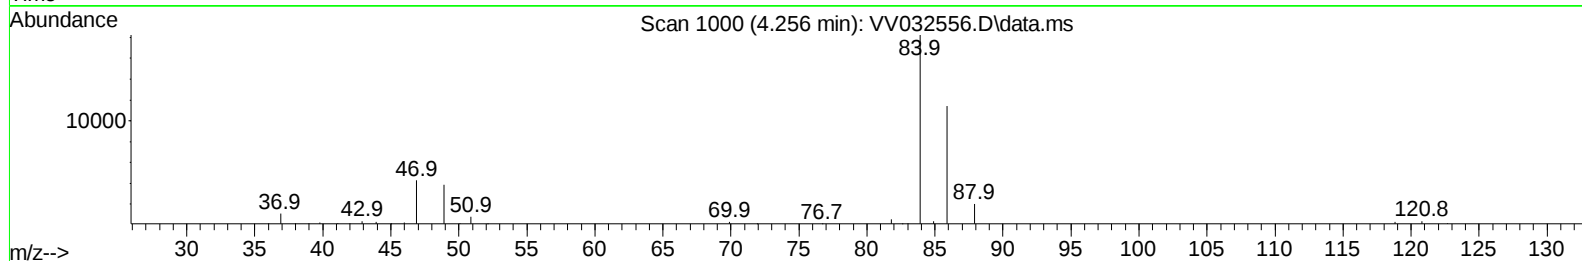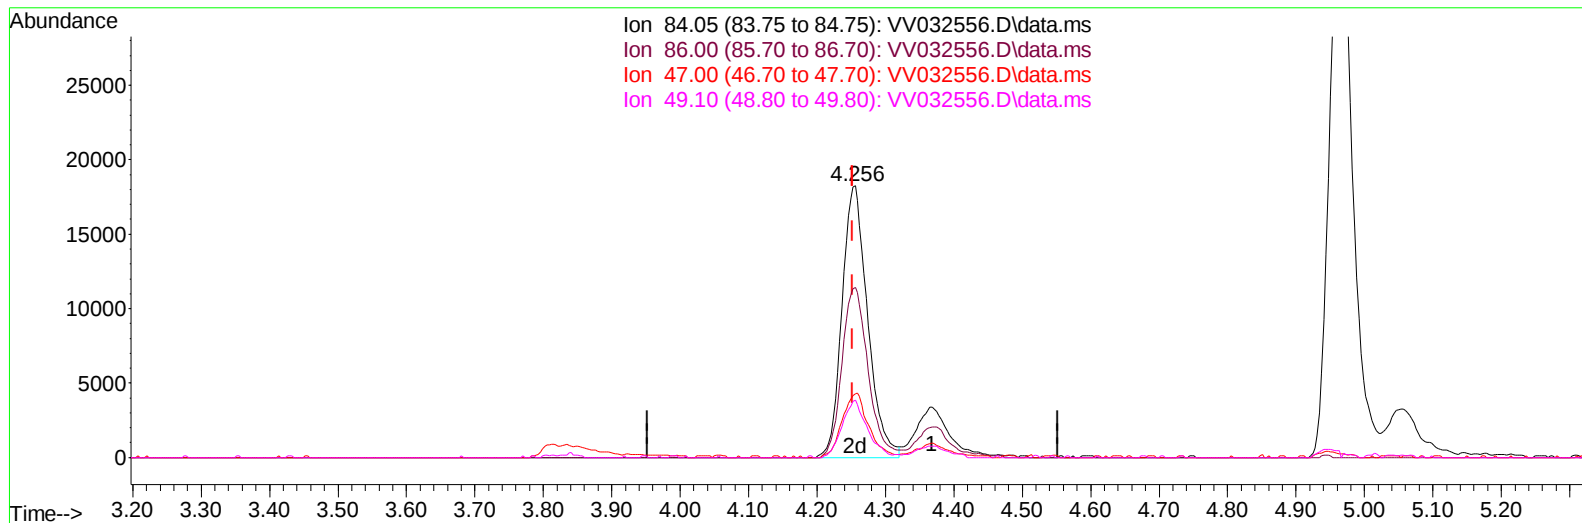

TIC: VV032556.D\data.ms

(24) Chloroform-d (S)

4.256min (+ 0.003) 4.47 ug/L m

response 47283

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	61.90	13.12#
47.00	43.10	6.97#
49.10	25.00	5.15#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032556.D
 Acq On : 21 Oct 2023 04:47
 Operator : SY/MD
 Sample : 04993-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX0

Manual IntegrationsAPPROVED

Quant Time: Oct 23 03:01:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 21 02:44:24 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
 Supervised By :Mahesh Dadoda 10/24/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.539	114		73707	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117		86057	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		38457	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		23463	3.914	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	78.200%	
7) Chloroethane-d5	1.532	69		23679	4.866	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	97.400%	
11) 1,1-Dichloroethene-d2	2.060	65		9553	3.779	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	75.600%	
20) 2-Butanone-d5	3.815	46		81247	53.578	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	107.160%	
24) Chloroform-d	4.256	84		47283m	4.471	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	89.400%	
26) 1,2-Dichloroethane-d4	4.947	65		26224	5.235	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	104.800%	
32) Benzene-d6	4.963	84		89424	3.531	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	70.600%	
36) 1,2-Dichloropropane-d6	5.992	67		30706	3.660	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	73.200%	
41) Toluene-d8	7.246	98		75245	3.250	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	65.000%#	
43) trans-1,3-Dichloroprop...	7.561	79		11033	3.711	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	74.200%	
46) 2-Hexanone-d5	8.030	63		64874	46.378	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	92.760%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		29115	4.961	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	99.200%	
66) 1,2-Dichlorobenzene-d4	11.564	152		30094	4.217	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	84.400%	
Target Compounds							
47) Tetrachloroethene	7.905	164		44949	7.166	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032556.D
Acq On : 21 Oct 2023 04:47
Operator : SY/MD
Sample : 04993-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Manual IntegrationsAPPROVED

Quant Time: Oct 23 03:01:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 21 02:44:24 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/23/2023
Supervised By :Mahesh Dadoda 10/24/2023

